

Exhibit 16




US 20030203493A1


(19) **United States**(12) **Patent Application Publication** (10) **Pub. No.: US 2003/0203493 A1**
Lemme et al. (43) **Pub. Date: Oct. 30, 2003**(54) **AUTOMATED MOLECULAR PATHOLOGY
APPARATUS HAVING FIXED SLIDE
PLATFORMS**(22) Filed: **Apr. 28, 2003****Related U.S. Application Data**(75) Inventors: **Charles Lemme**, Tucson, AZ (US);
Devon Campbell, Tucson, AZ (US);
Andrew Ghusson, Tucson, AZ (US);
David Bryant, Tucson, AZ (US); **Kurt
Reinhardt**, Tucson, AZ (US); **William
Richards**, Tucson, AZ (US); **Vincent
Rizzo**, Tucson, AZ (US); **Wayne
Showalter**, Tucson, AZ (US)(60) Provisional application No. 60/375,679, filed on Apr.
26, 2002.**Publication Classification**(51) **Int. Cl.⁷** **G01N 35/00**; G01N 1/31
(52) **U.S. Cl.** **436/46**; 422/100; 422/64;
436/180


Correspondence Address:

Norman P. Soloway
HAYES SOLOWAY PC
130 W. Cushing Street
Tucson, AZ 85701 (US)(73) Assignee: **Ventana Medical Systems, Inc.**(21) Appl. No.: **10/424,372**(57) **ABSTRACT**

Apparatus and methods for automatically staining or treating multiple tissue samples mounted on slides are provided, in which the slides and reagent bottles are held in fixed position, and the reagent, wash and coverslipping solutions brought to the slides. Alternatively, the slides are held in fixed position, while the reagent, wash and coverslipping solutions brought to the slides.

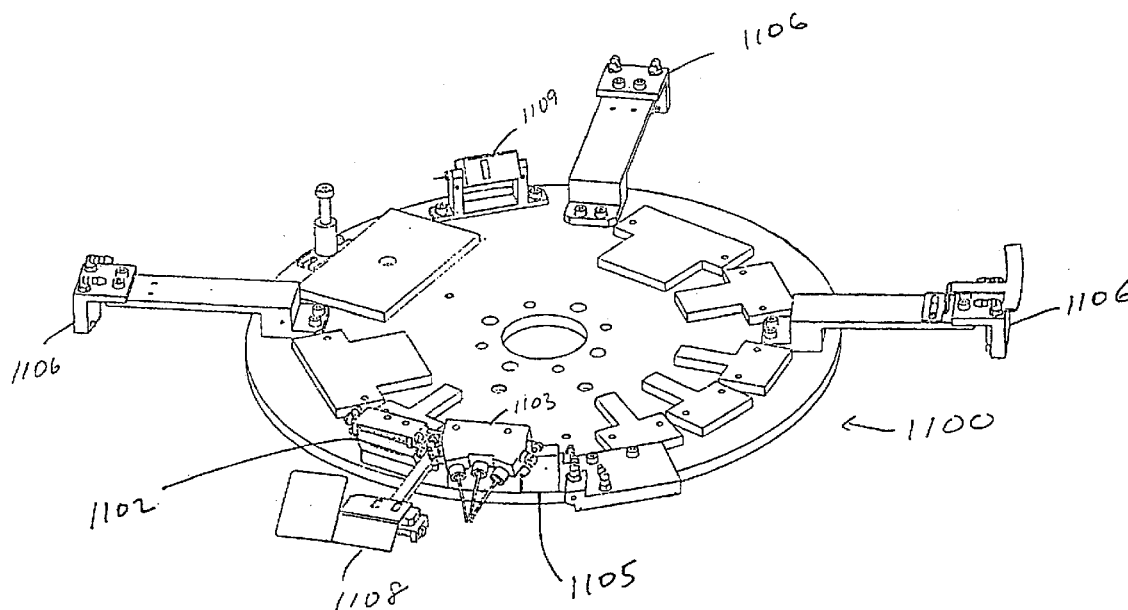

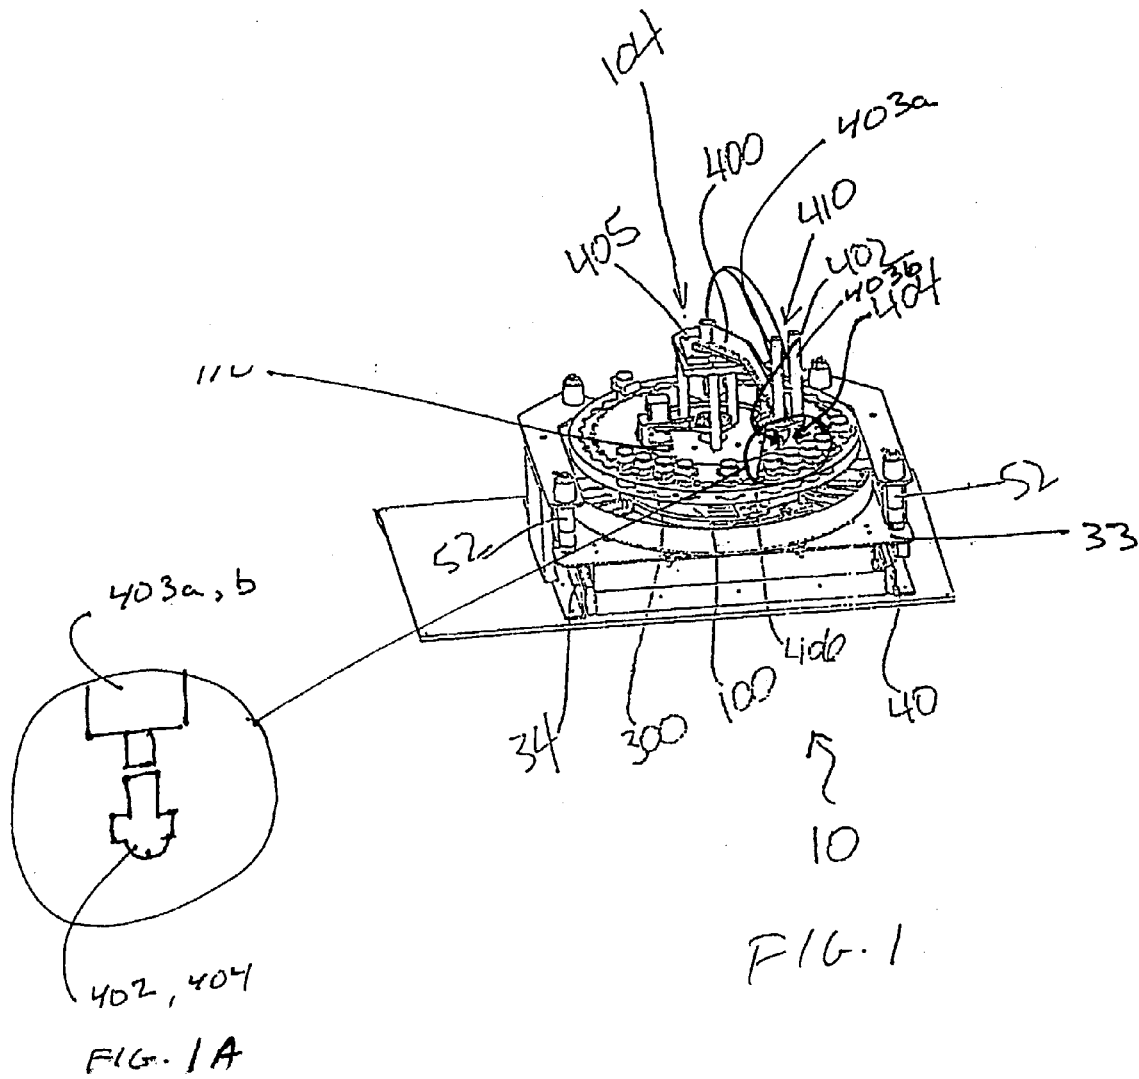

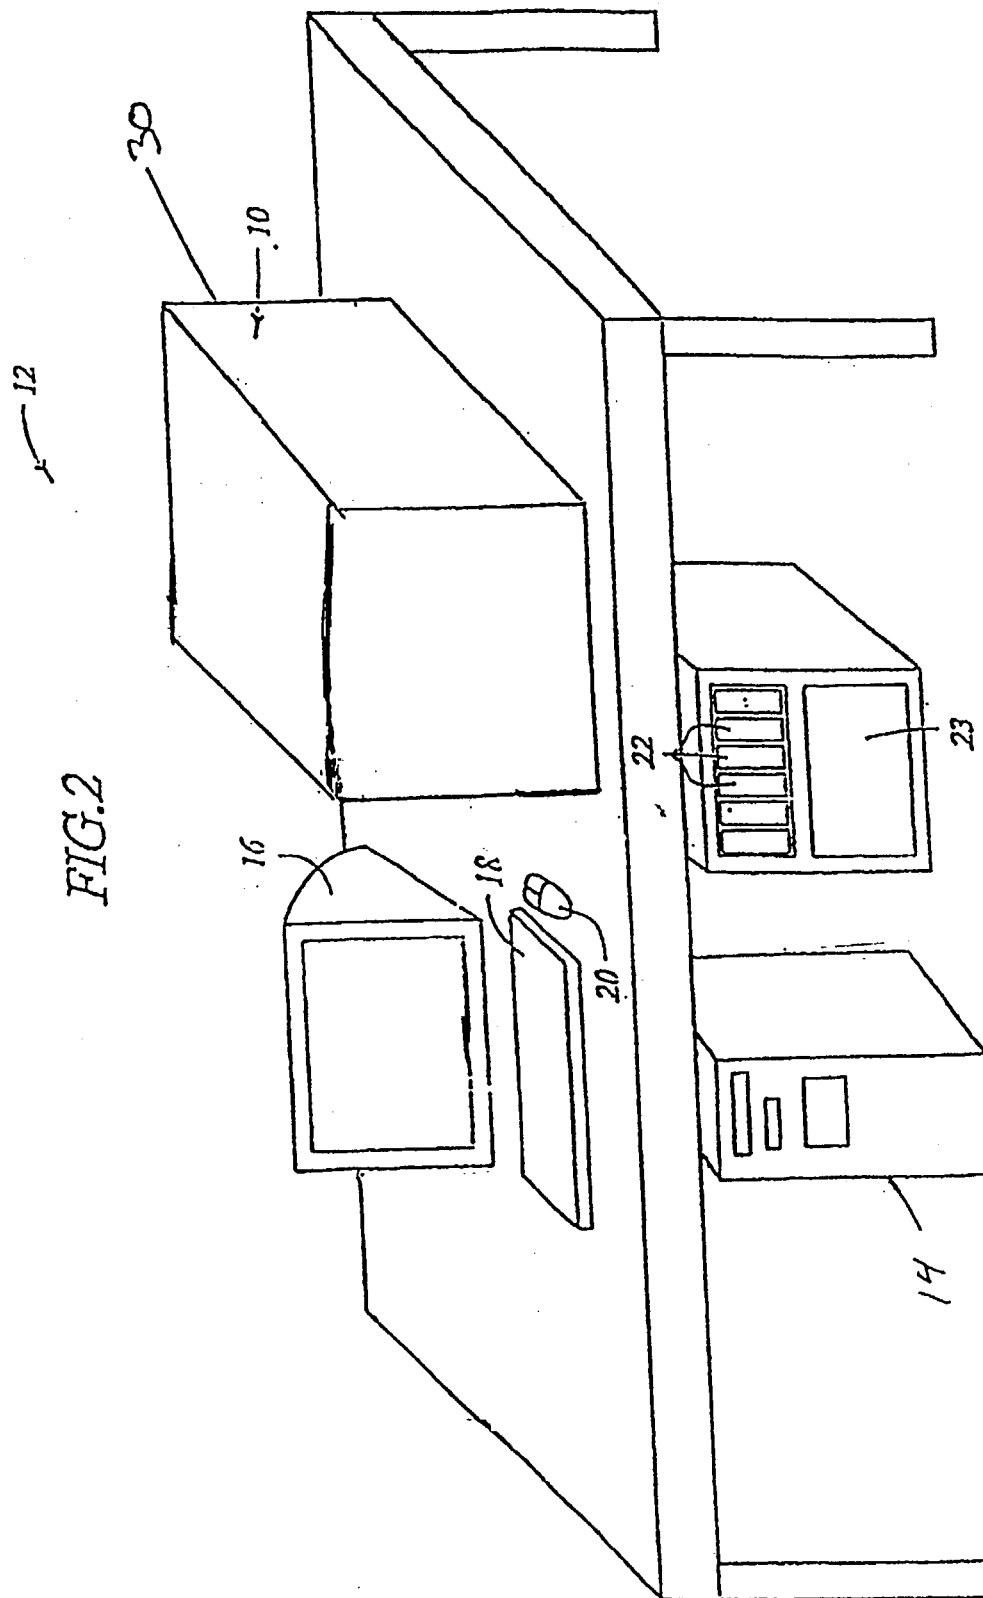

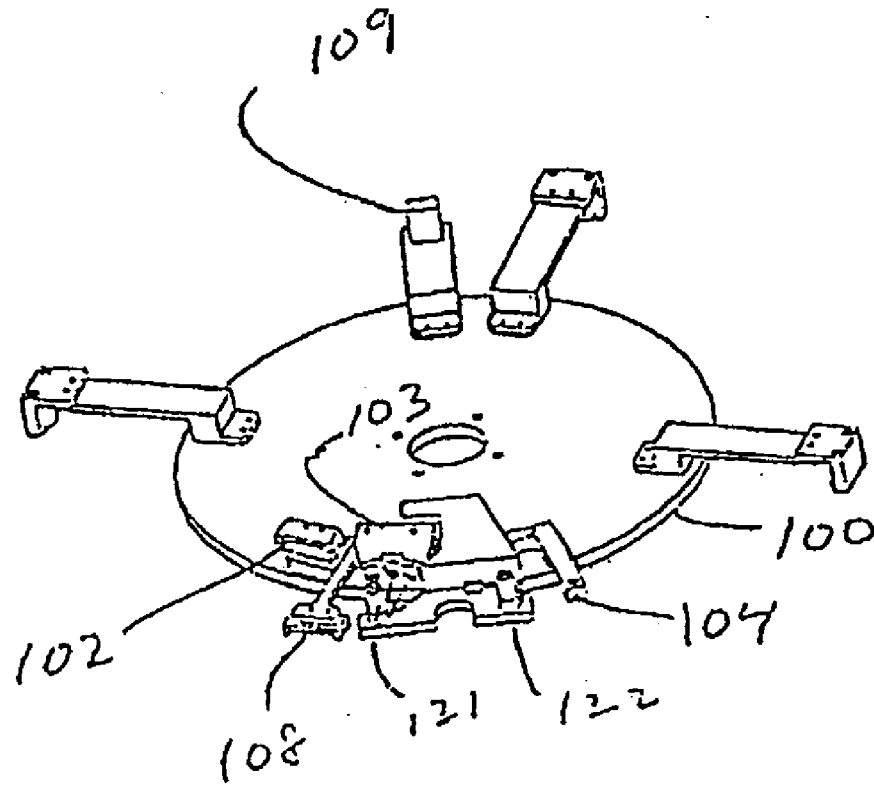


FIG. 3

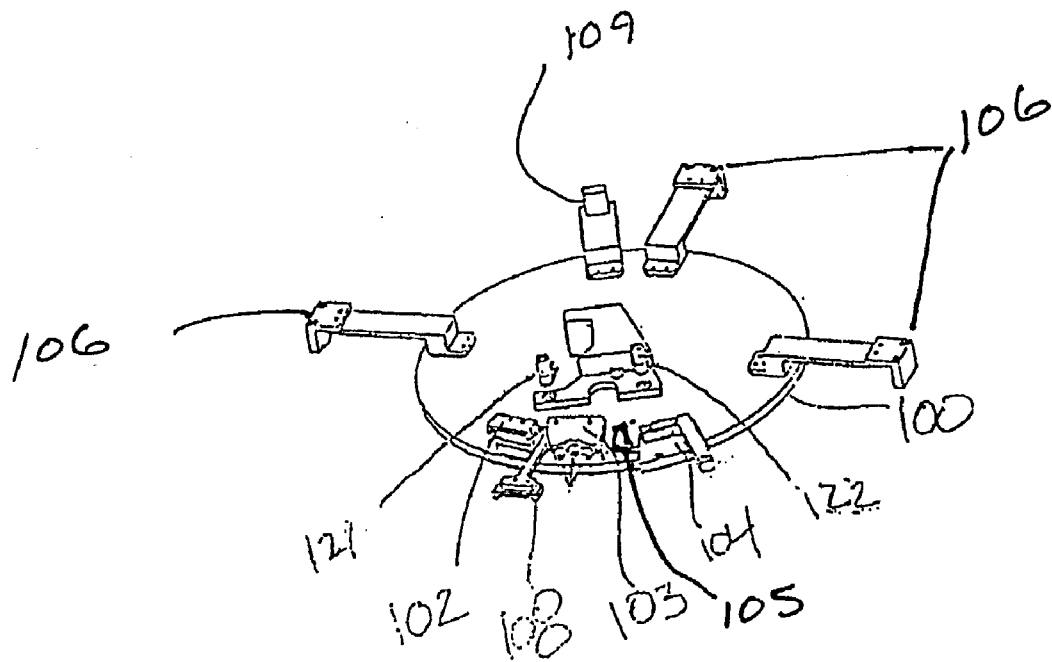


FIG. 3 A

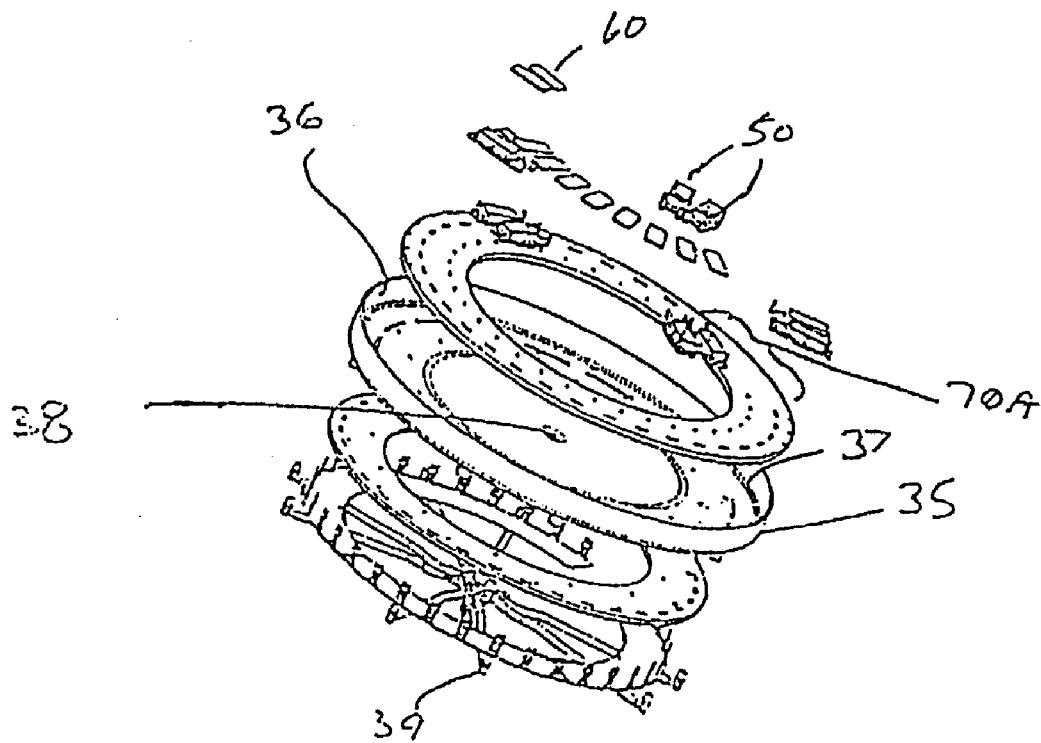


FIG. 4


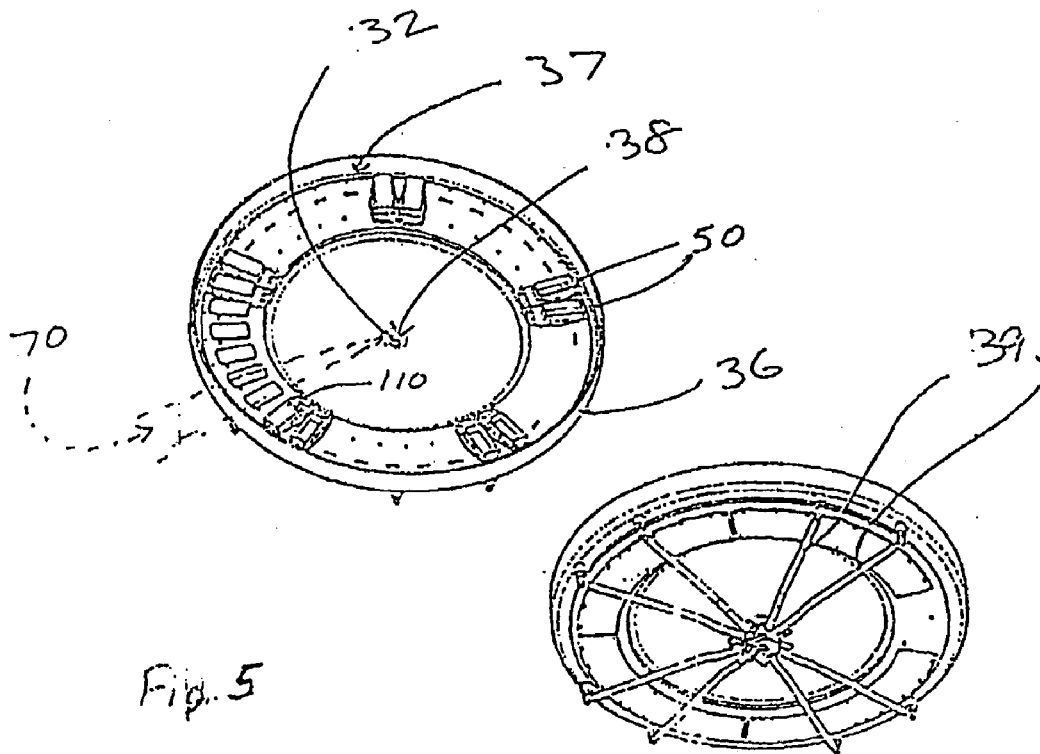


Fig. 5

Fig. 6

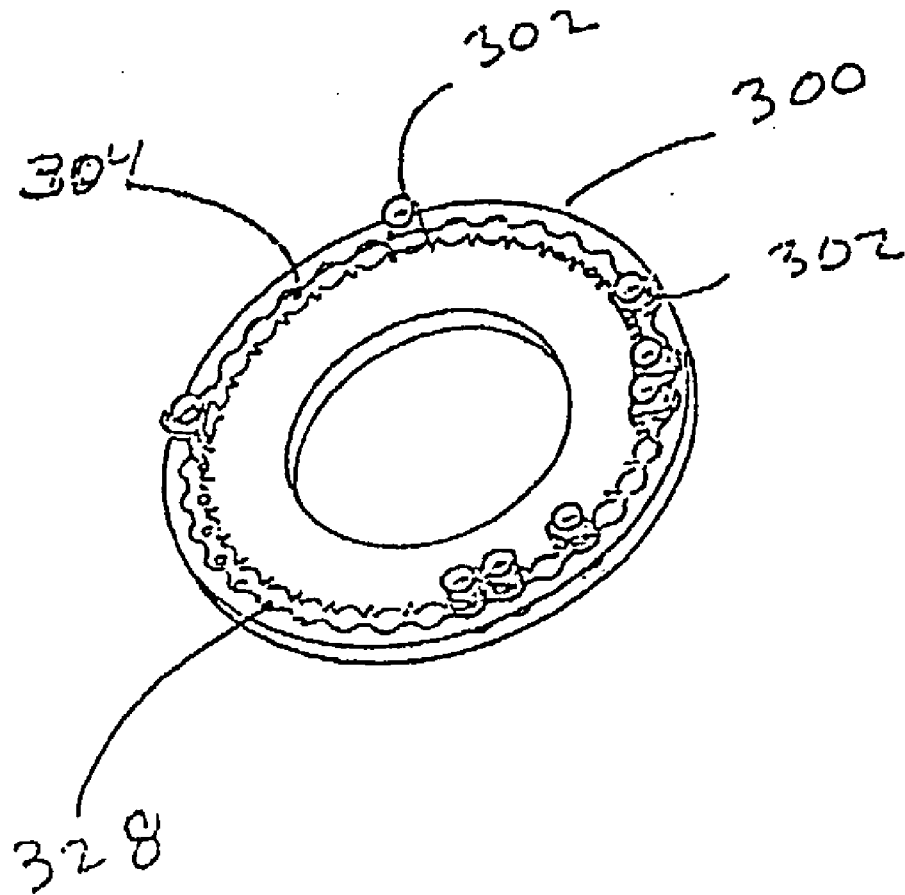

F167

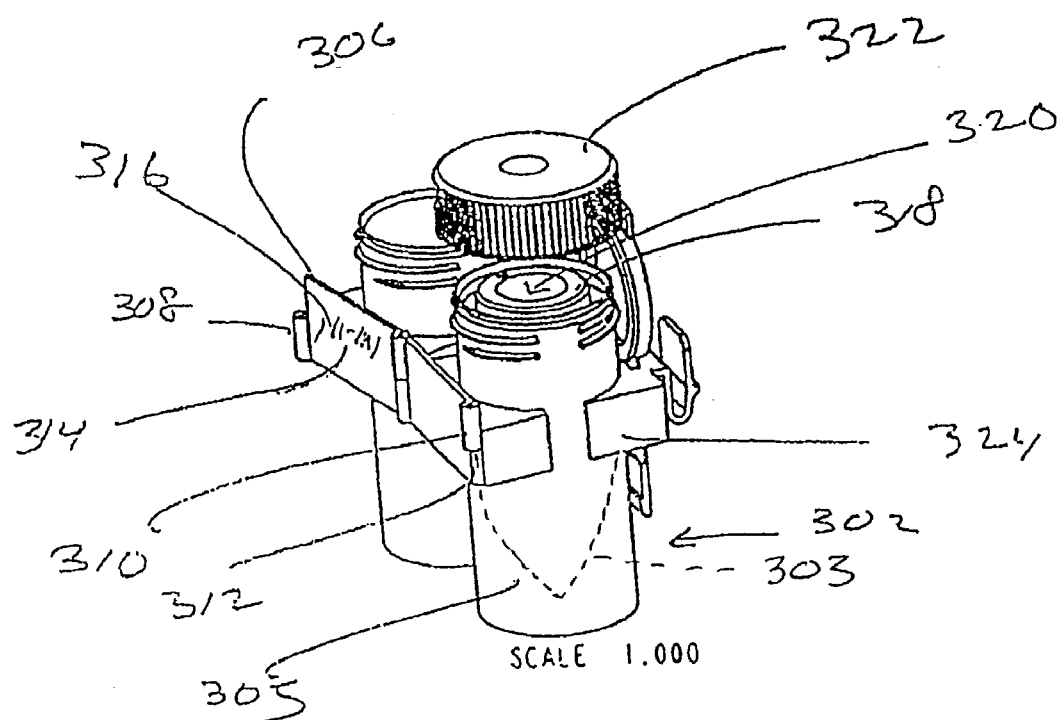


FIG. 8

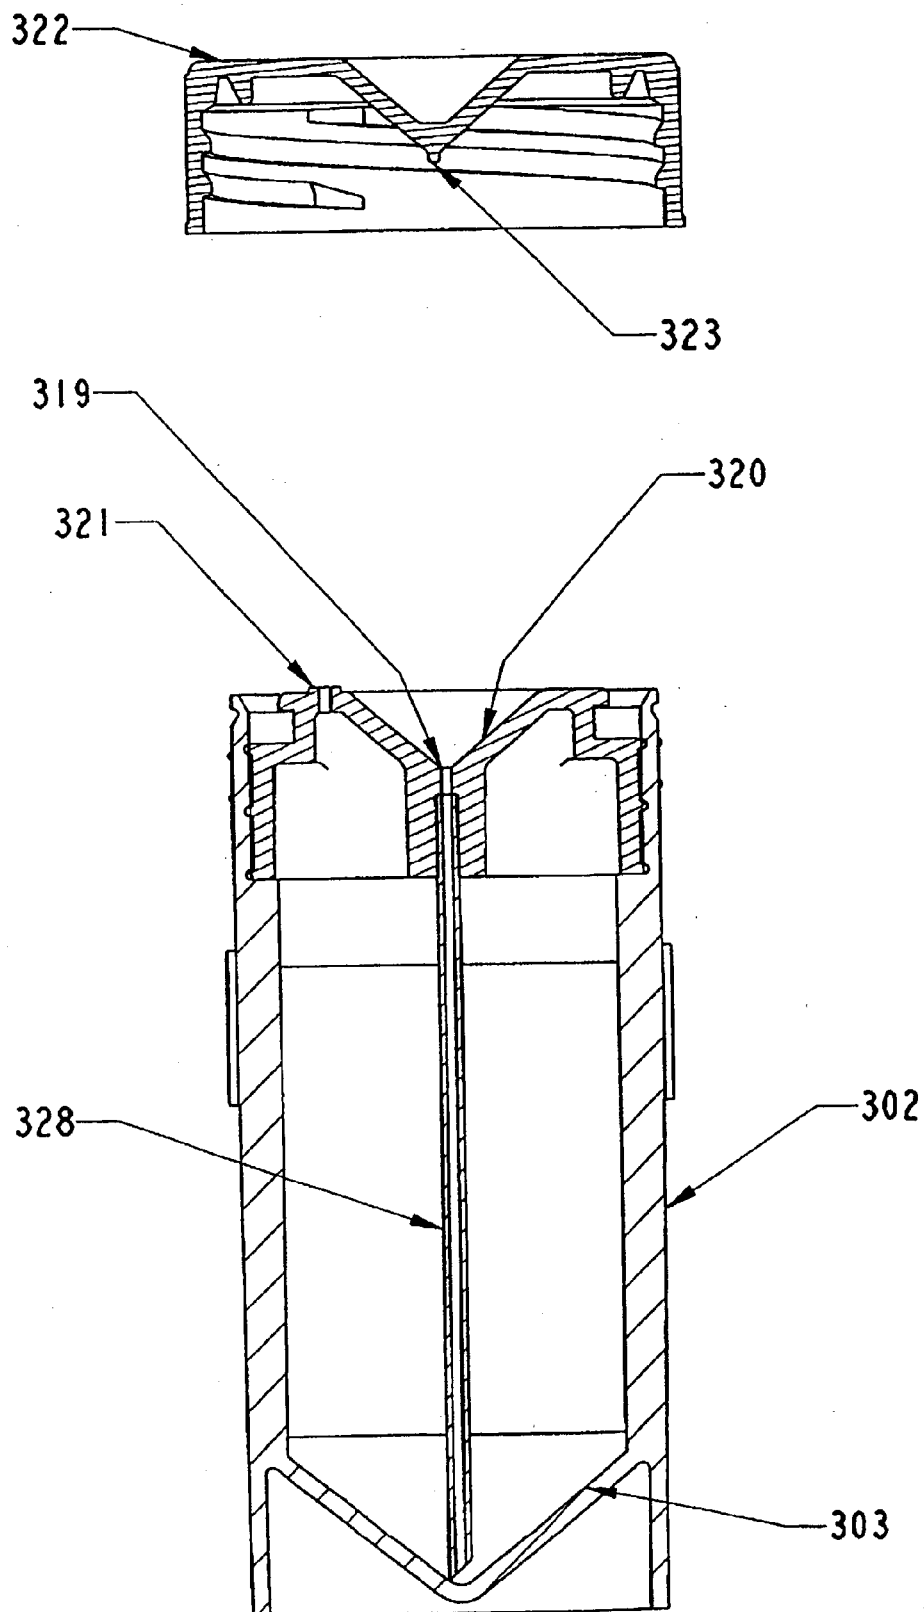


Figure 8A

Patent Application Publication Oct. 30, 2003 Sheet 10 of 22 US 2003/0203493 A1

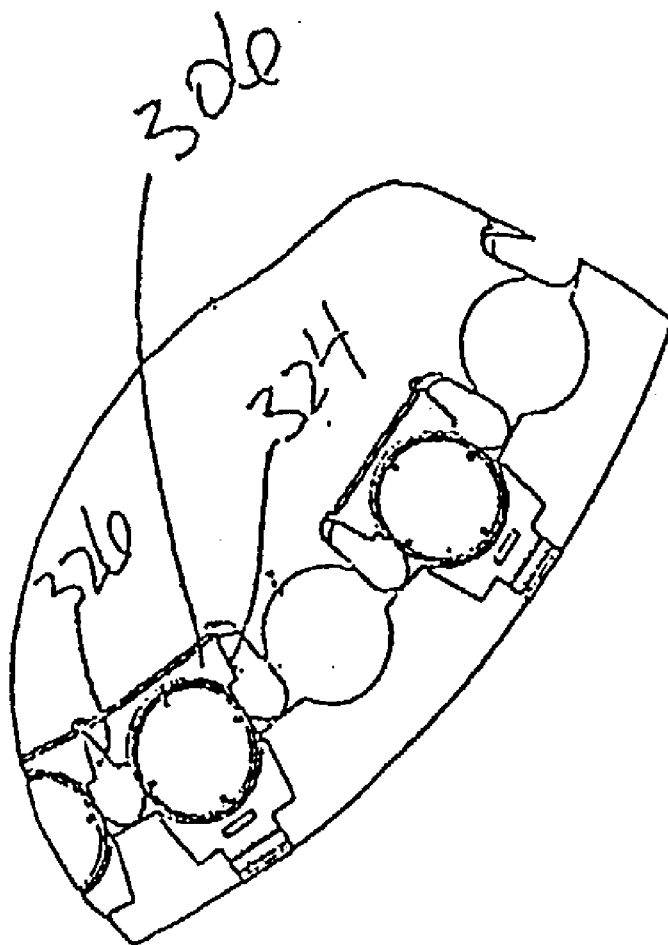


FIG. 9

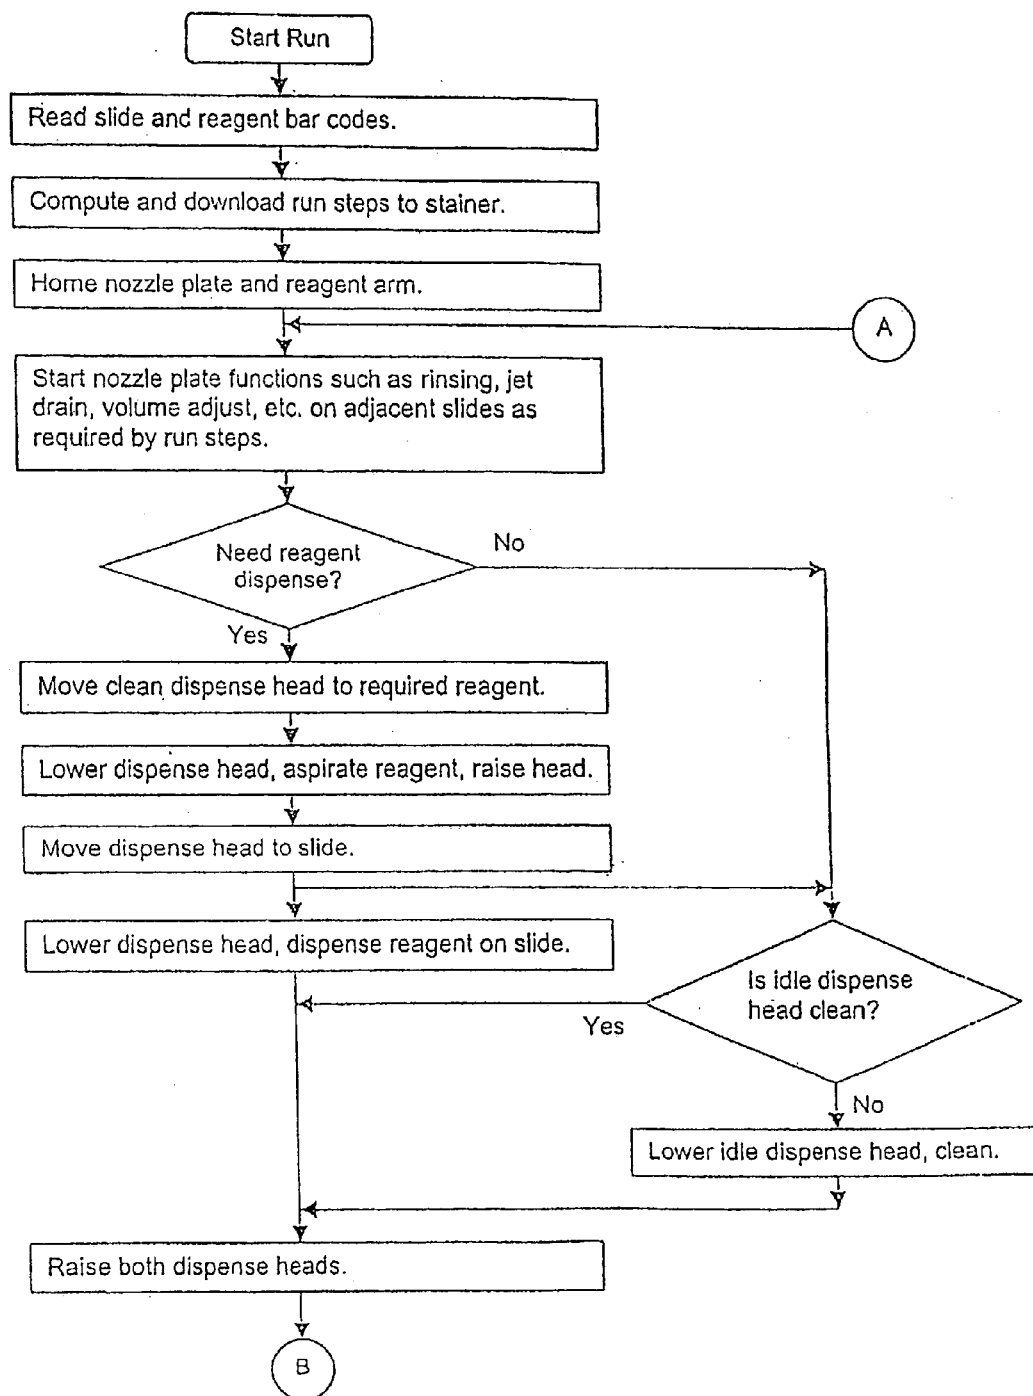


FIG. 10A



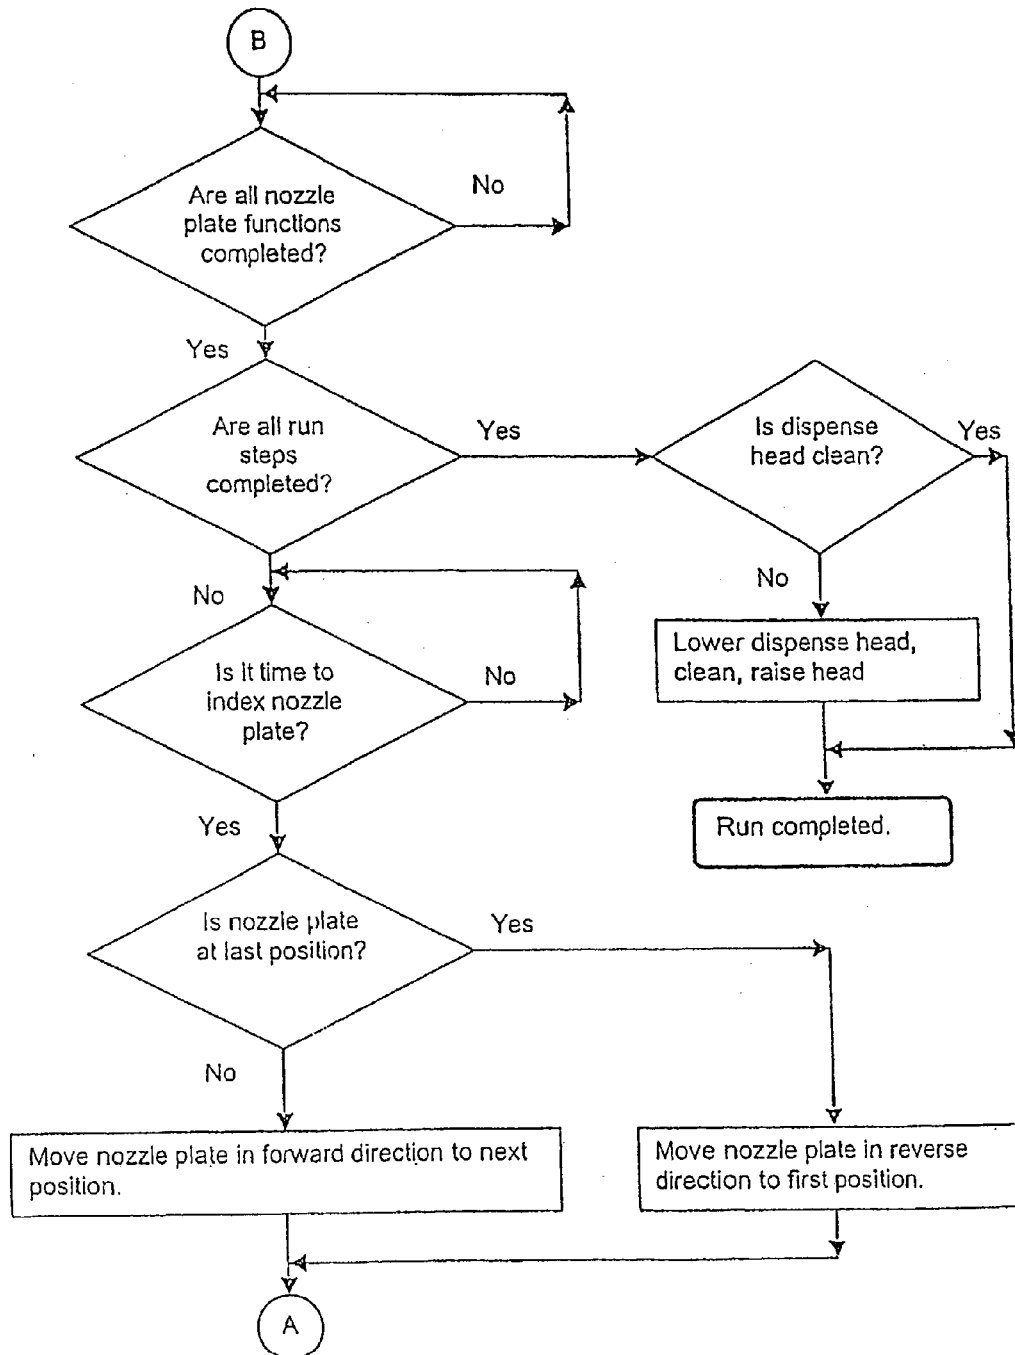


FIG. 10B

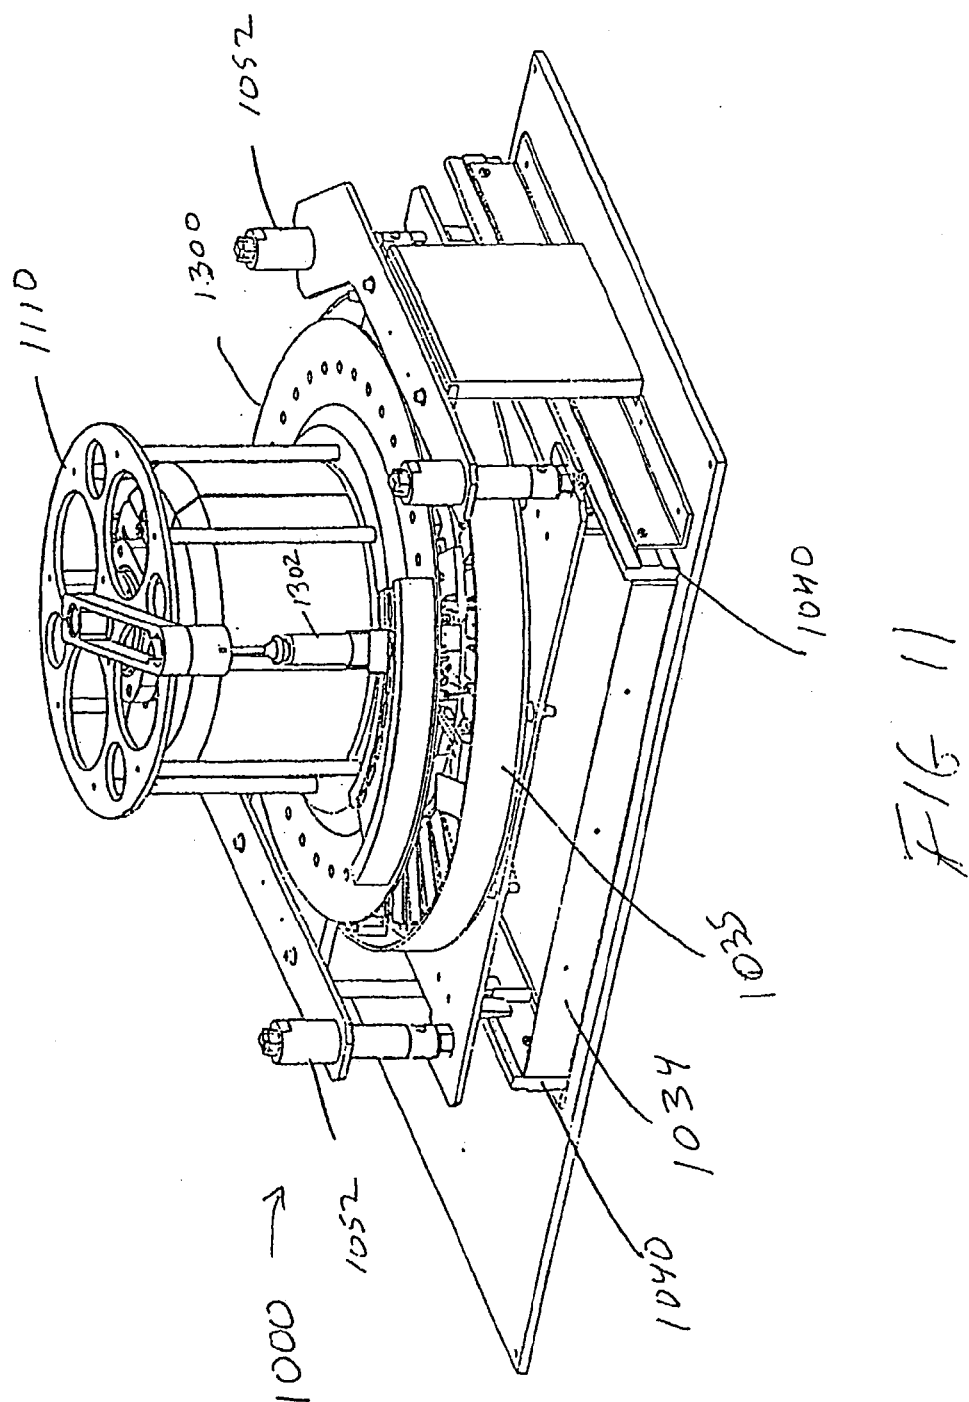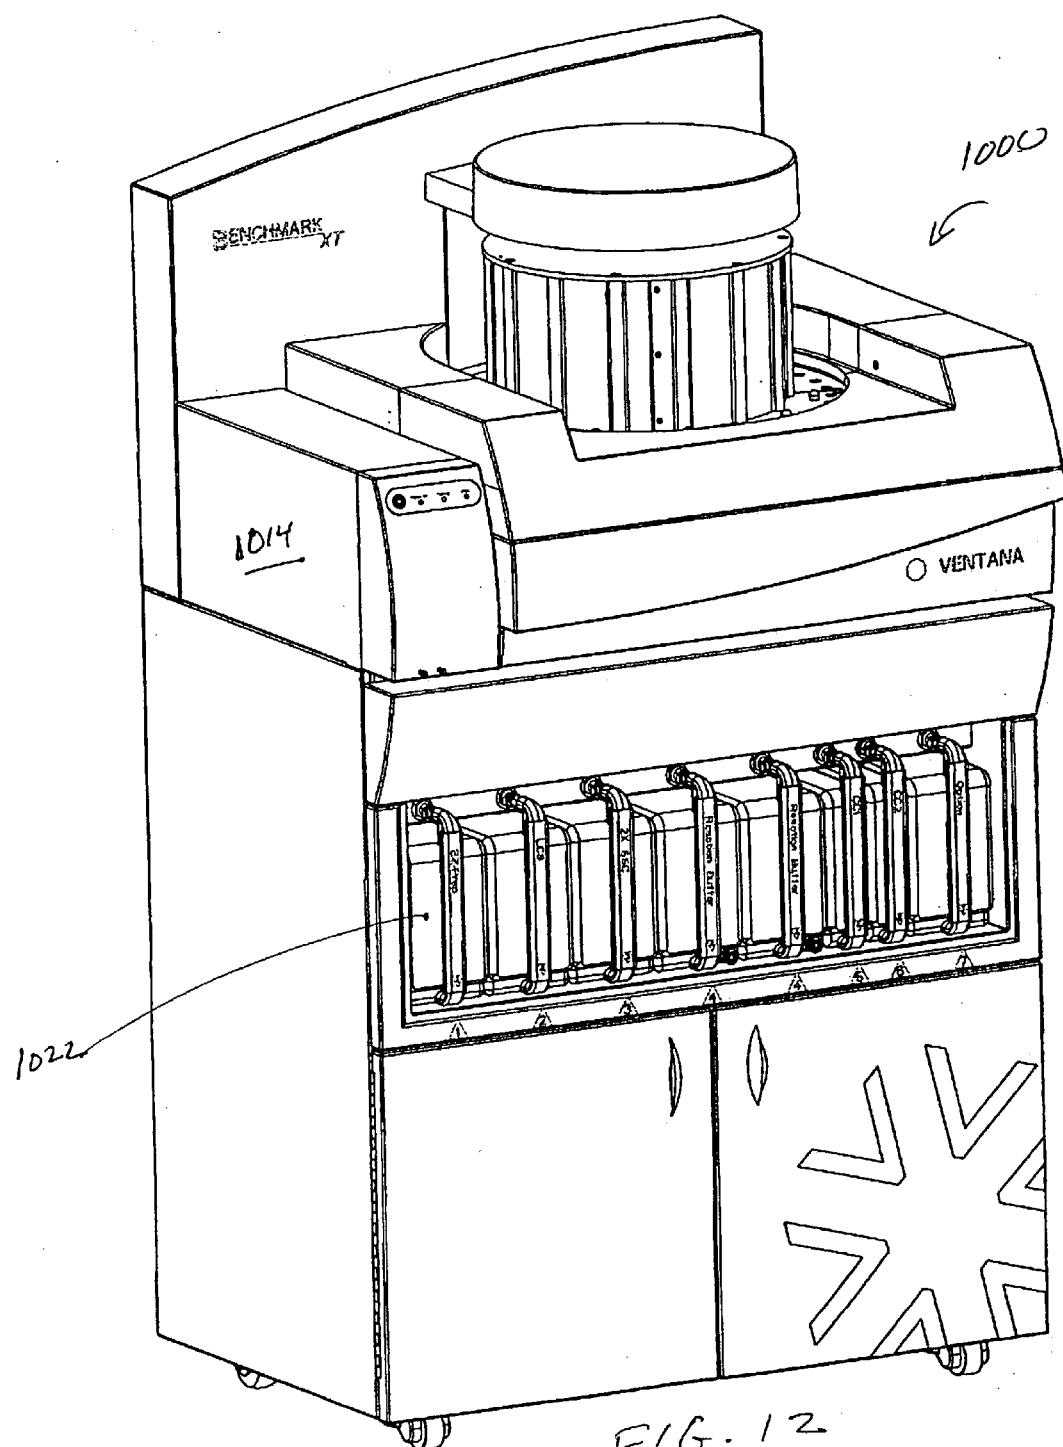

Patent Application Publication Oct. 30, 2003 Sheet 14 of 22 US 2003/0203493 A1



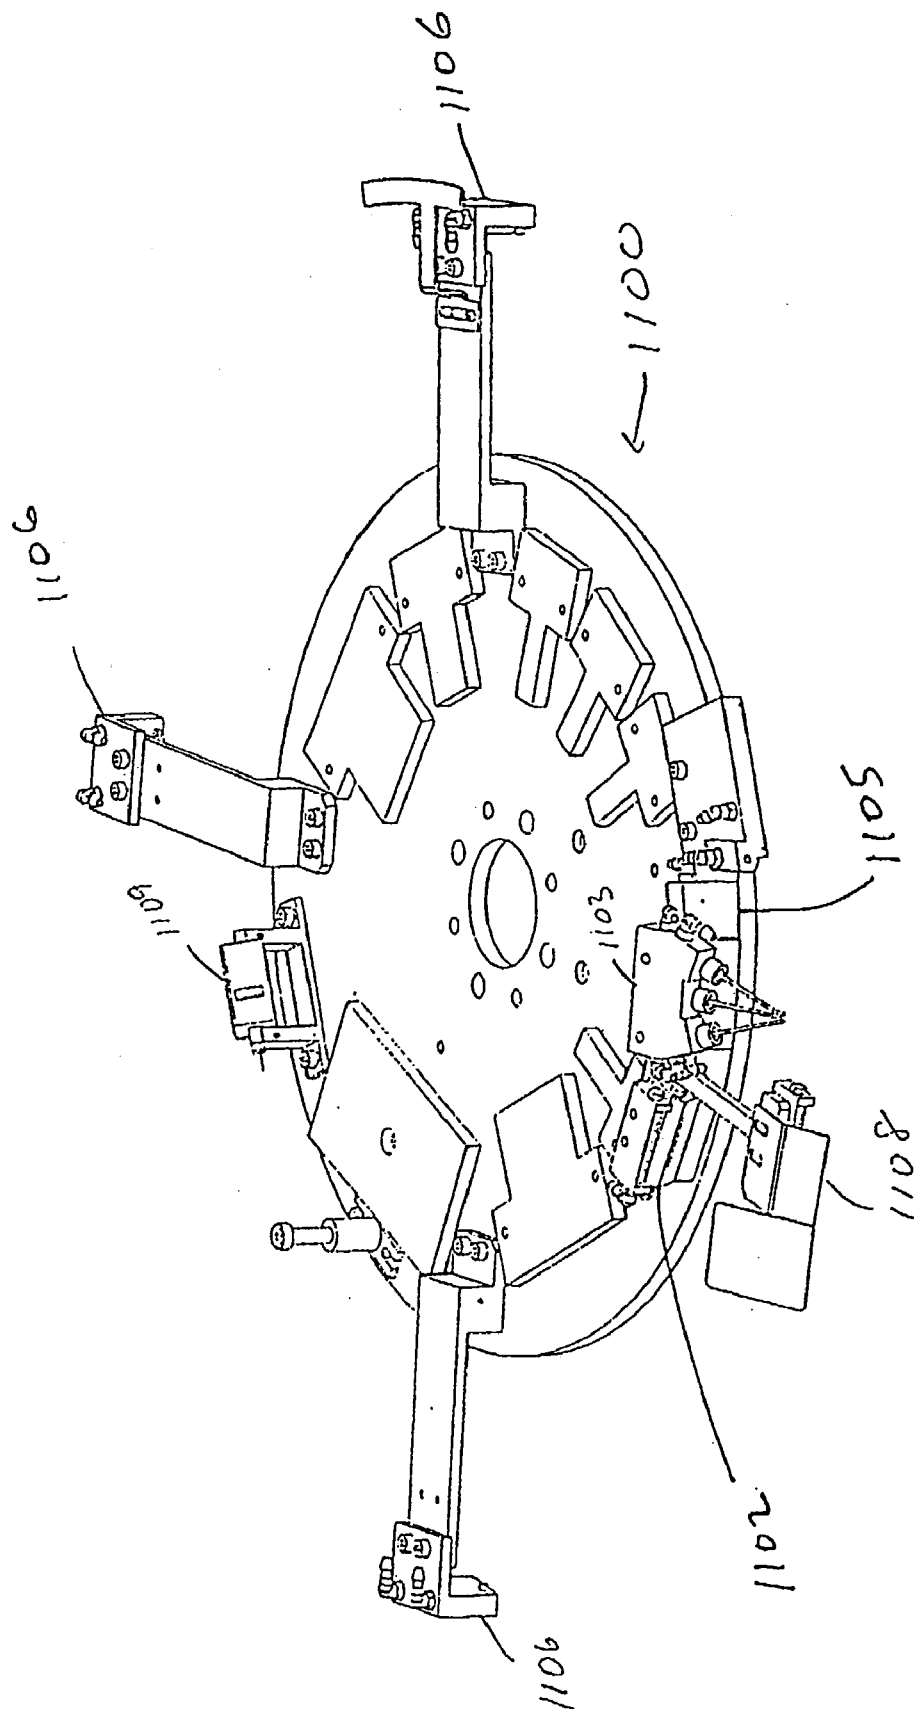
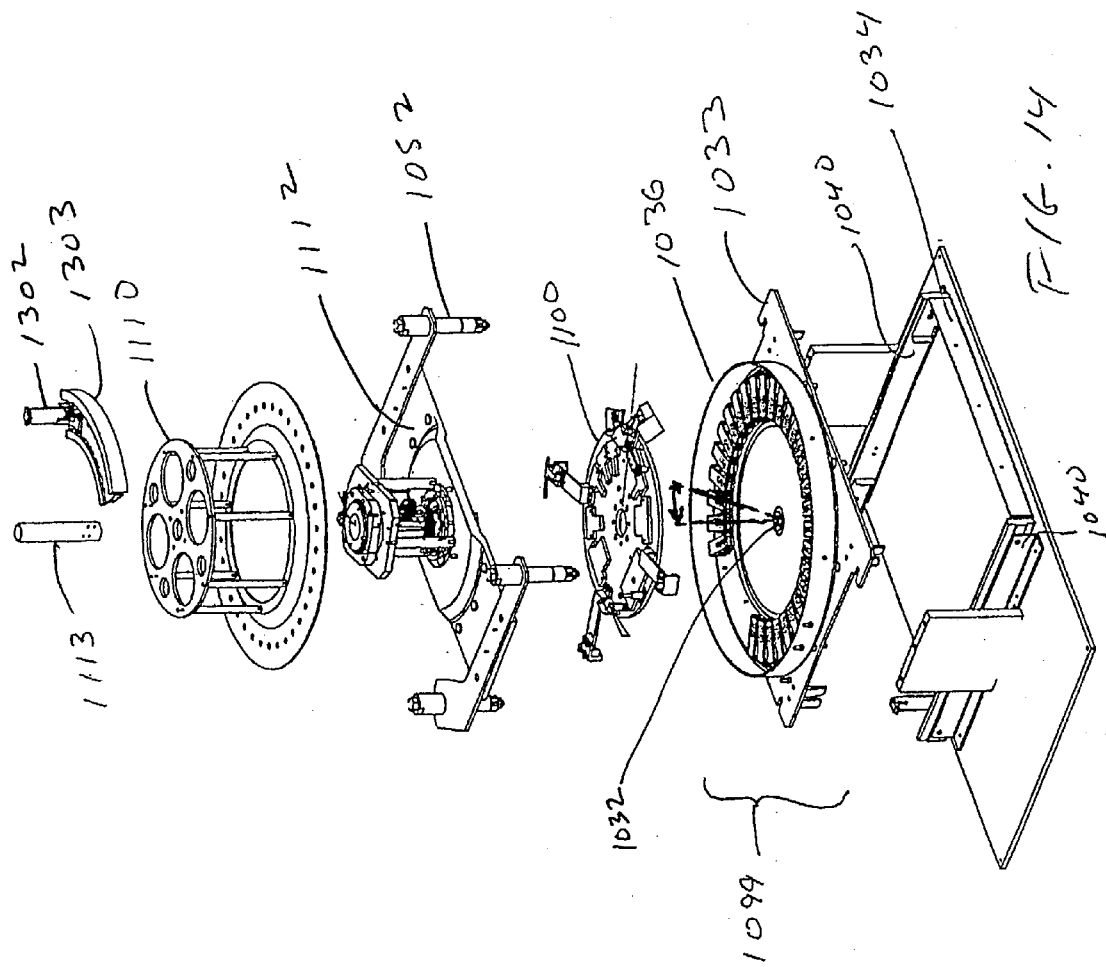


FIG. 13



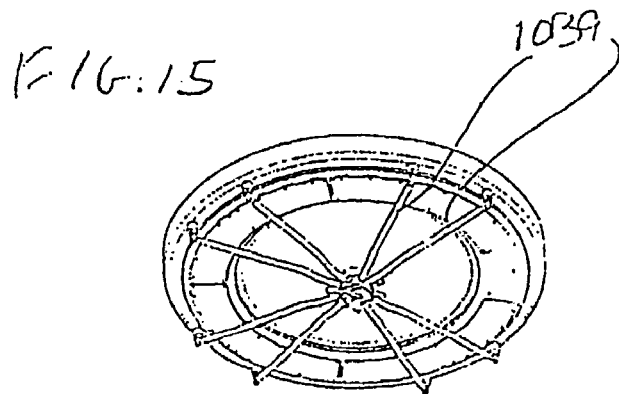
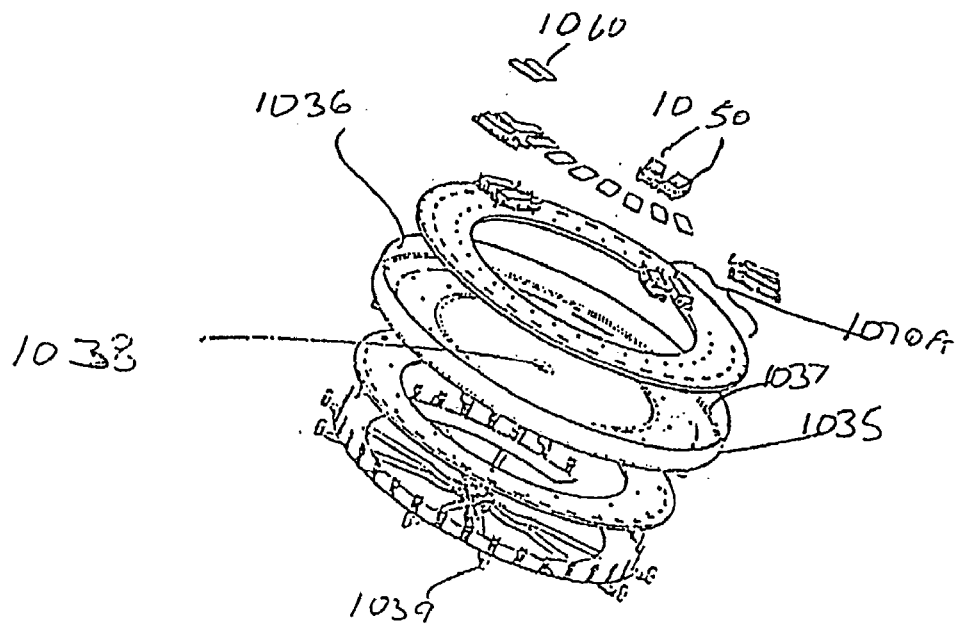


FIG. 16

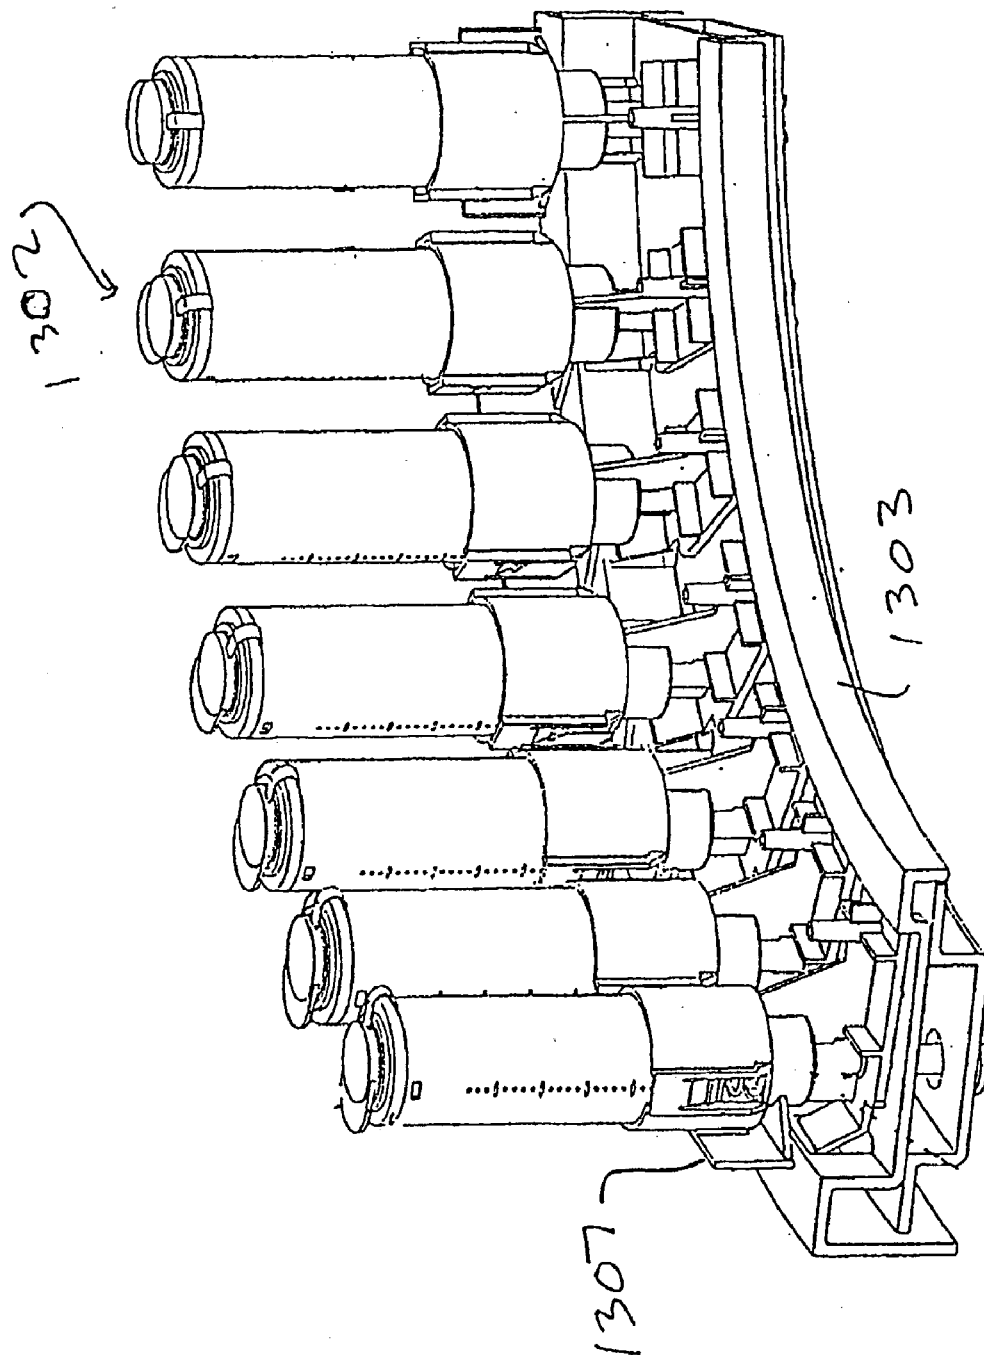


FIG. 17A

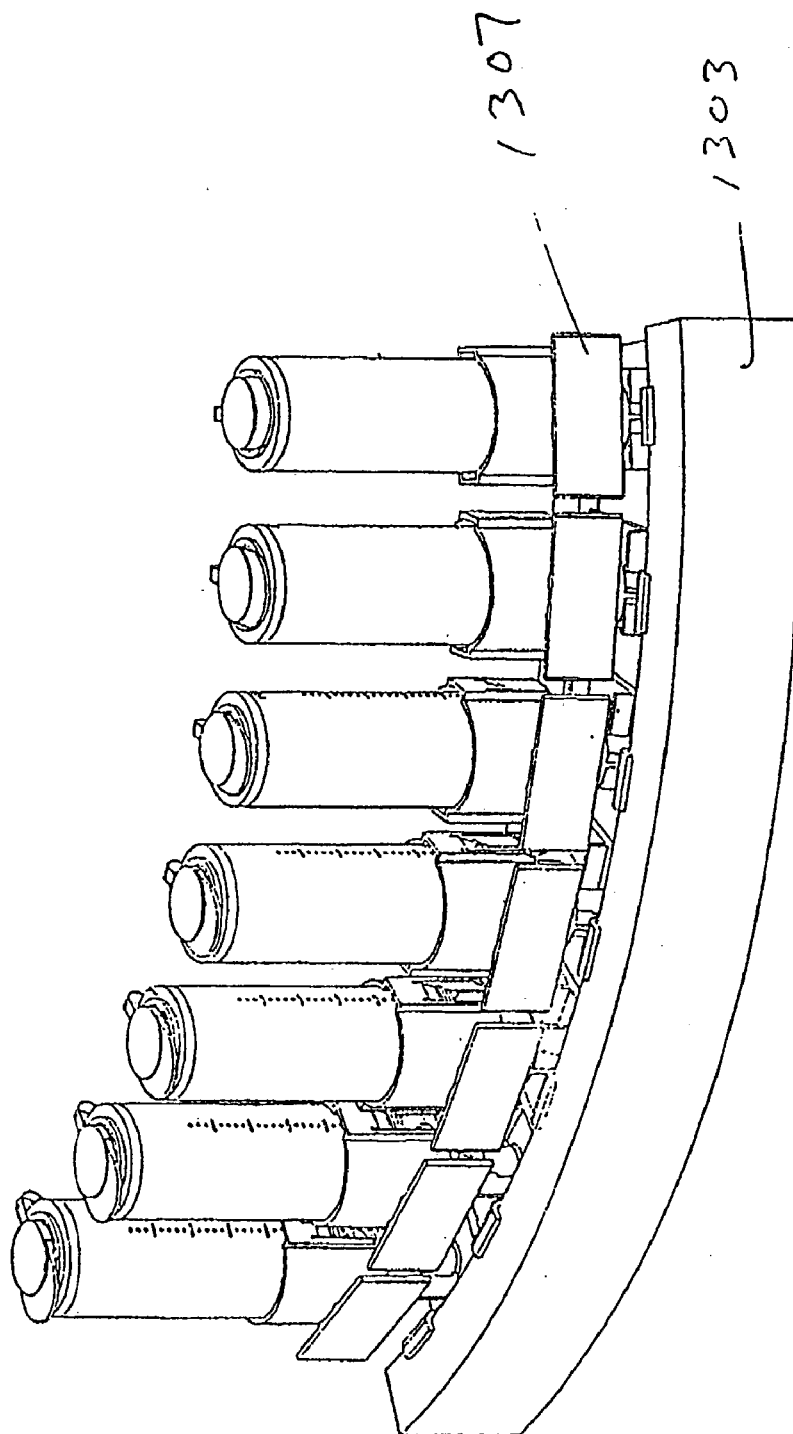


FIG. 17B

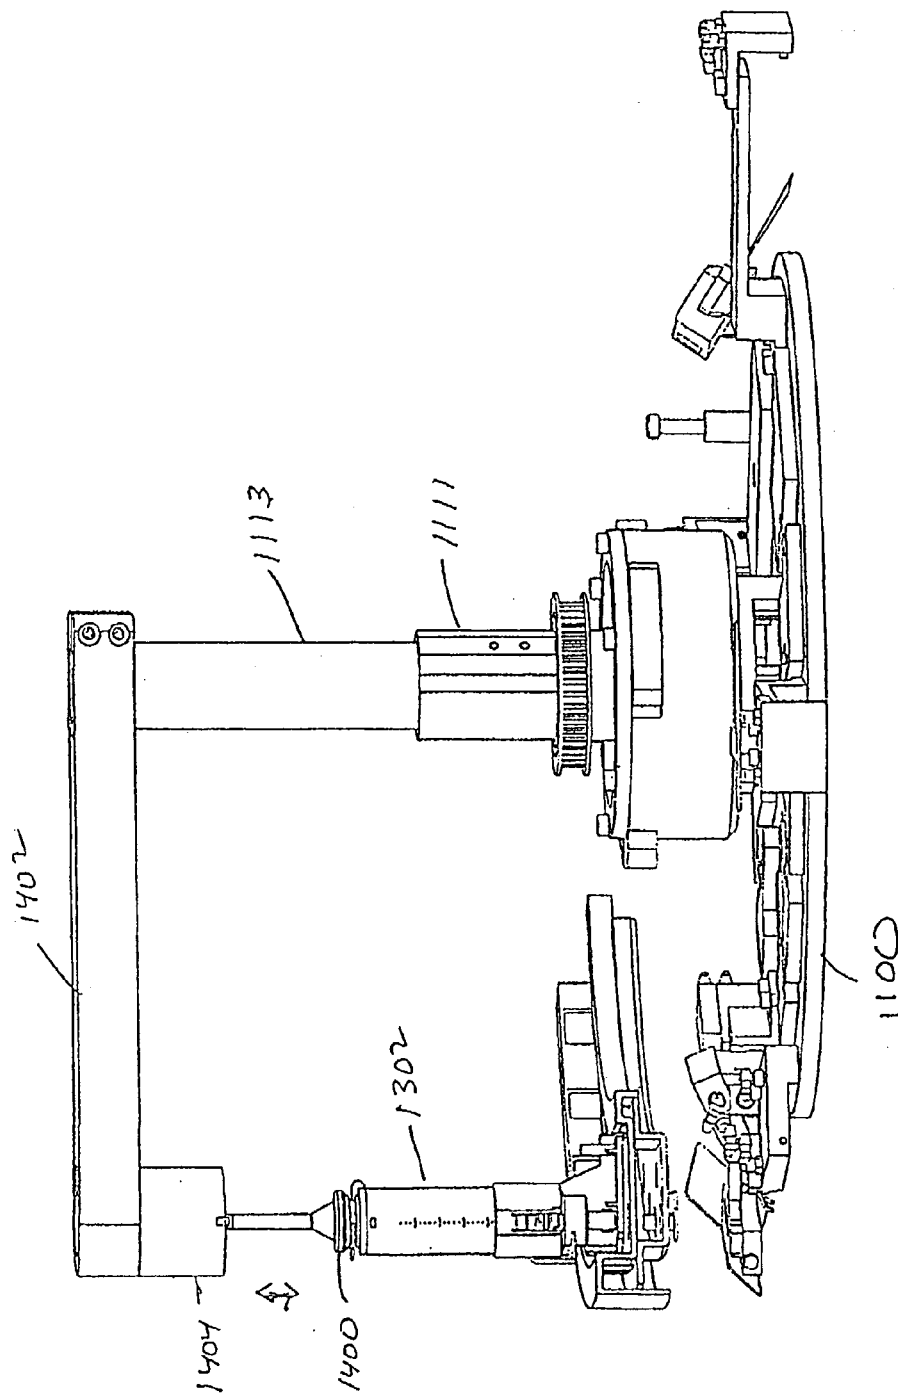


FIG. 18

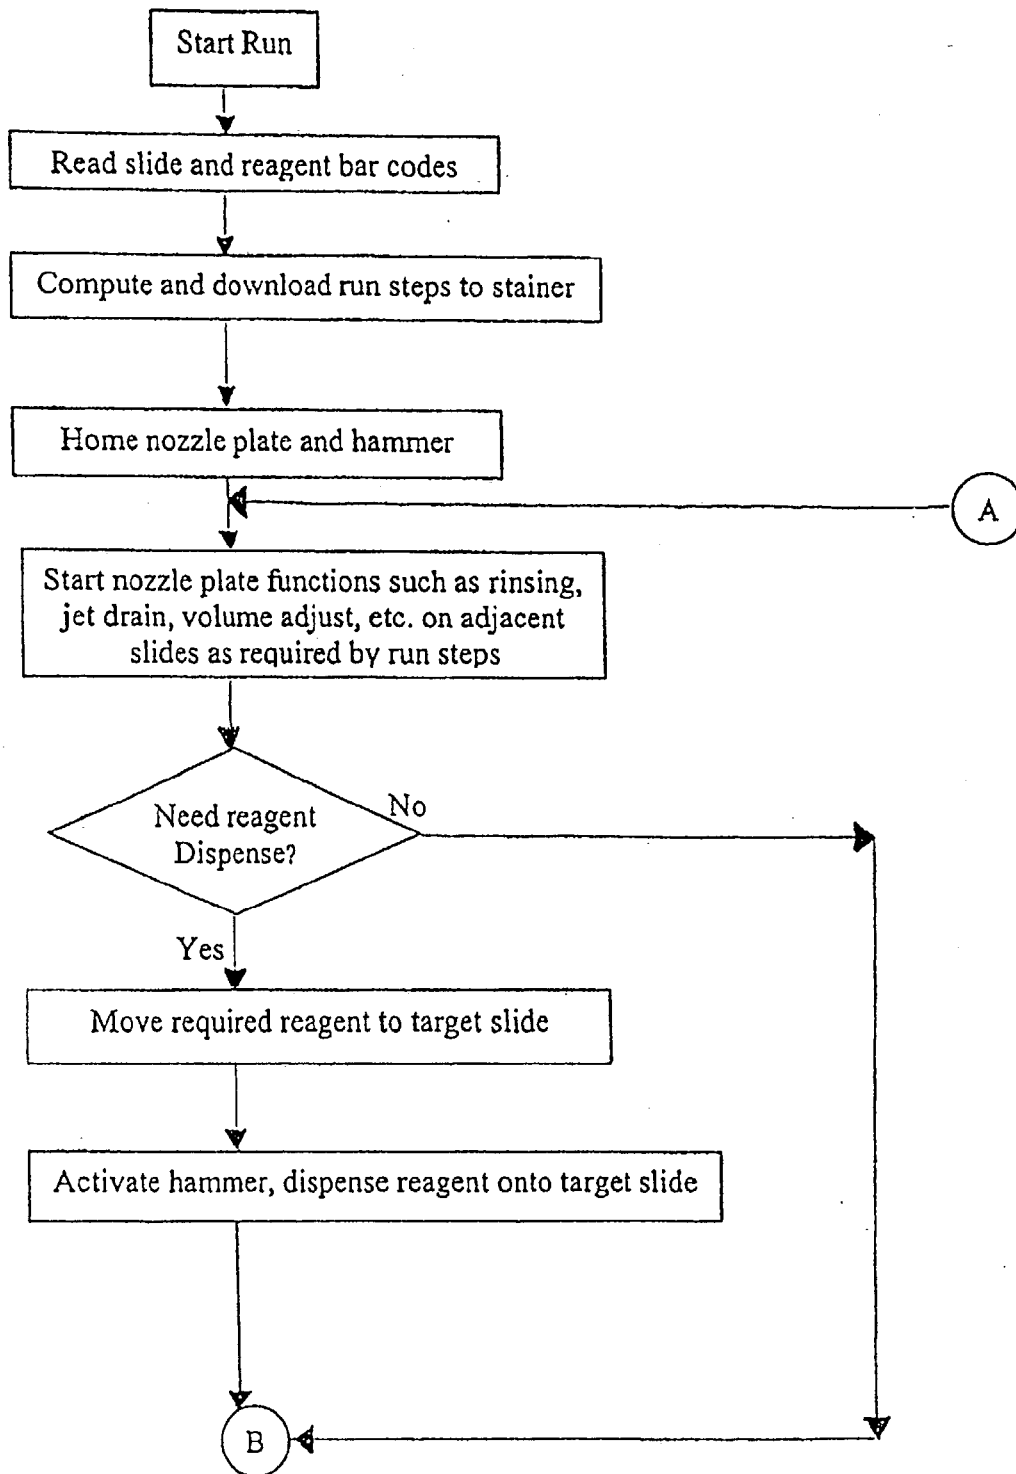


FIG. 19A

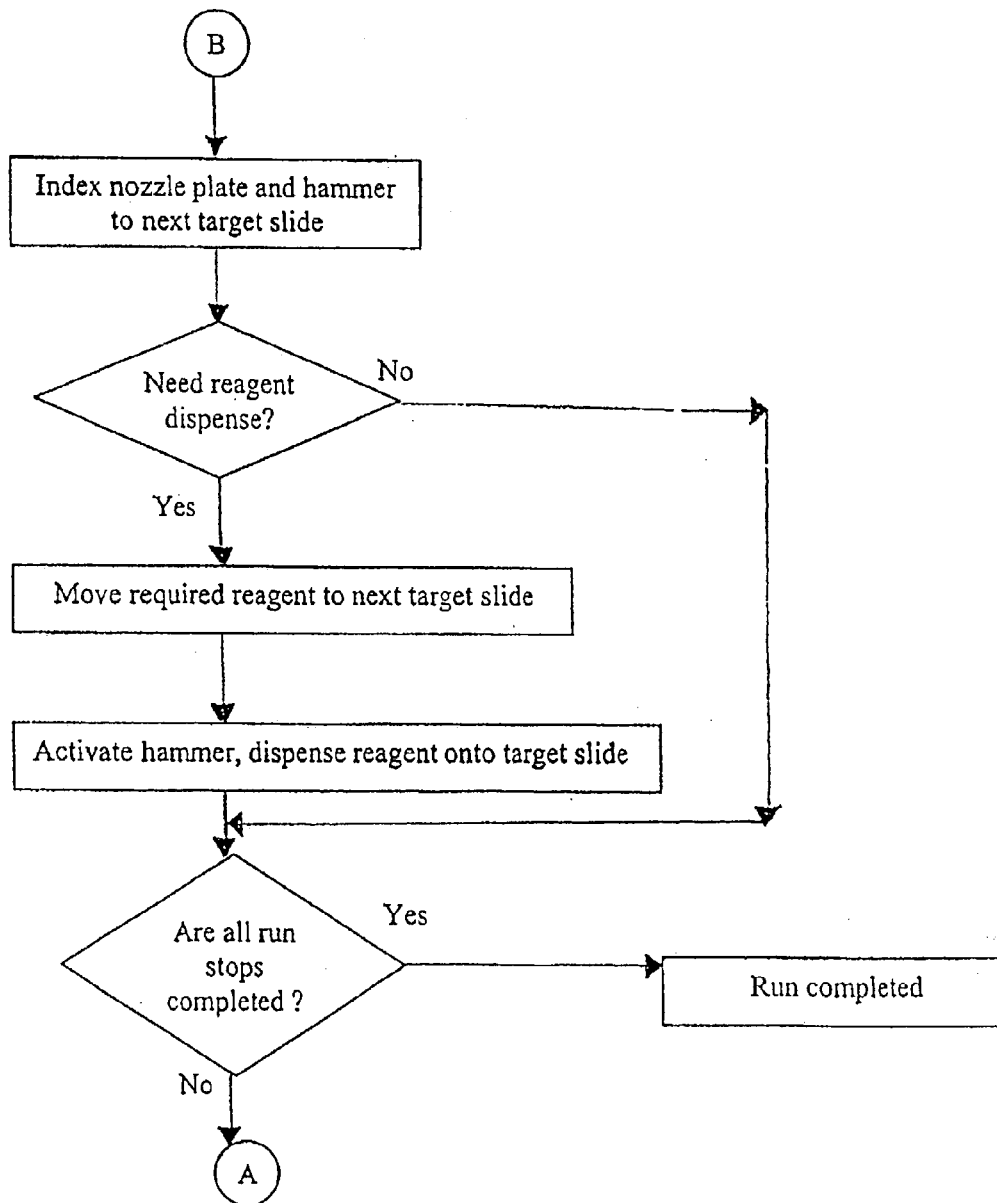


FIG. 19B

US 2003/0203493 A1

Oct. 30, 2003

1

AUTOMATED MOLECULAR PATHOLOGY APPARATUS HAVING FIXED SLIDE PLATFORMS

CROSS REFERENCE TO RELATED APPLICATION

[0001] This Application claims benefit of priority from U.S. Provisional Application Serial No. 60/375,679 filed Apr. 26, 2002.

FIELD OF THE INVENTION

[0002] The present invention is directed to apparatus for use in diagnostic molecular pathology and, more particularly, to such apparatus used for the automated staining and/or treating of tissue samples mounted on microscope slides.

BACKGROUND OF THE INVENTION

[0003] Molecular pathology is the examination at a molecular level of the DNA, mRNA, and proteins that cause or are otherwise associated with disease. From this examination important information about patient diagnosis, prognosis, and treatment options can be elucidated. The practice of molecular pathology is generally divided into two main areas: (i) analysis of DNA, mRNA, and proteins in intact cells (in-situ), and (ii) analysis of these biological materials after they have been extracted from tissues. The first category, to which the present invention is primarily directed, has the advantage that it allows the pathologist or scientist to study the histopathologic architecture or morphology of the tissue specimen under the microscope at the same time that the nucleic acid or proteins are being assayed. These techniques include immunohistochemistry (IHC) which looks at proteins, in-situ hybridization (ISH) which looks at nucleic acids, histochemistry (HC) which looks at carbohydrates, and enzyme histochemistry (EHC) which looks at enzyme chemistry. For example, ISH can be used to look for the presence of a genetic abnormality or condition such as amplification of cancer causing genes specifically in cells that, when viewed under a microscope, morphologically appear to be malignant. ISH is also useful in the diagnosis of infectious diseases as it allows detection not only of a microbial sequence but also of precisely which cells are infected. This may have important clinicopathologic implications and is an effective means to rule out the possibility that positive hybridization signal may have come from an adjacent tissue of no clinical concern or from blood or outside contamination.

[0004] IHC utilizes antibodies which bind specifically with unique epitopes present only in certain types of diseased cellular tissue. IHC requires a series of treatment steps conducted on a tissue section or cells (e.g. blood or bone marrow) mounted on a glass slide to highlight by selective staining certain morphological indicators of disease states. Typical steps include pretreatment of the tissue section to remove the paraffin and reduce non-specific binding, retrieval of antigens or cell conditioning masked by cross-linking of the proteins from the chemical fixatives, antibody treatment and incubation, enzyme-labeled secondary antibody treatment and incubation, substrate reaction with the enzyme to produce a fluorophore or chromophore highlighting areas of the tissue section having epitopes binding with the antibody, counterstaining, and the like. Most of these

steps are separated by multiple rinse steps to remove unreacted residual reagent from the prior step. Incubations can be conducted at elevated temperatures, usually around 37° C., and the tissue must be continuously protected from dehydration. ISH analysis, which relies upon the specific binding affinity of DNA or RNA probes with unique or repetitive nucleotide sequences from the cells of tissue samples or bodily fluids, requires a similar series of process steps with many different reagents and is further complicated by varying temperature requirements.

[0005] In view of the large number of repetitive treatment steps needed for both IHC and ISH, automated systems have been introduced to reduce human labor and the costs and error rate associated therewith, and to introduce uniformity. Examples of automated systems that have been successfully employed include the ES®, NexES®, DISCOVERY™, BENCHMARK™ and Gen II® staining Systems available from Ventana Medical Systems (Tucson, Ariz.). These systems employ a microprocessor-controlled system including a revolving carousel supporting radially positioned slides. A stepper motor rotates the slide carousel placing each slide under one of a series of reagent dispensers positioned above the slides. As described in U.S. Pat. No. 6,352,861 B1, bar codes on the slides and reagent dispensers fully automate the computer-controlled actuation of the dispensers onto the slides so that different reagent treatments can be performed for each of the various tissue samples.

[0006] Instrumentation such as the Ventana Medical Systems ES®, Gen II® NexES®, BENCHMARK® and DISCOVERY® systems are fundamentally designed to sequentially apply reagents to tissue sections mounted on one by three inch glass microscope slides under controlled environmental conditions. The instrument must perform several basic functions such as reagent application, washing (to remove a previously applied reagent), jet draining (a technique to reduce the residual buffer volume on a slide subsequent to washing), Liquid Coverslip™ application (a light oil application used to contain reagents and prevent evaporation), and other instrument functions.

[0007] The Ventana Medical Systems staining instruments mentioned above process slides on a rotating slide carousel. The instrumentation described herein has the slides fixed in a stationary position and rotates the basic processing stations above the fixed slides. The following details of how the slides are processed, the process algorithm, is the same regardless of the physical configuration.

[0008] The process of staining tissue on a slide consists of the sequential repetition of the basic instrument functions described above. Essentially a reagent is applied to the tissue then incubated for a specified time at a specific temperature. When the incubation time is completed the reagent is washed off the slide and the next reagent is applied, incubated, and washed off, etc, until all of the reagents have been applied and the staining process is complete.

[0009] It is desirable to permit any staining protocol for any of the slides being run, i.e. any combination of reagents and incubation times. In addition, to stain multiple slides as quickly as possible the instrument should process the slides simultaneously. This is feasible given that most of the time slides are just incubating, thus freeing up time to perform the washing, reagent application and other functions on other slides.

US 2003/0203493 A1

Oct. 30, 2003

2

[0010] One algorithm to accomplish simultaneous staining (sometimes referred to as the "random access" method) is to create a task and time schedule for each slide in the run, then perform each task on each slide when the schedule calls for it. The problem with this method is that incubation times will not be accurate if the instrument is busy performing a task on one slide when it is time to be washing another slide (thereby completing incubation on that slide). The variation in incubation times will be unpredictable since the total number of slides and the slide protocols vary.

[0011] Slide processing using a lock-step algorithm insures that all incubation times are accurate and predictable irrespective of the number of slides processed or the variation in slide protocols. While incubation times are assured, the lock step algorithm implies that incubation times must be an increment of the fundamental incubation time period. For example, with an incubation cycle of two minutes, the total incubation times must be multiples of two, i.e., two, four, six, eight etc. minutes in duration. However, the preferred embodiment of the present invention uses a four minute incubation time. Generally this is not a particular limitation since typical incubation times are an order of magnitude longer than the fundamental incubation period.

[0012] Prior art staining systems typically include either convection or radiation to warm the samples above laboratory ambient temperatures for steps requiring elevated temperatures. Heating the slide improves staining quality by acceleration of the chemical reaction and can permit a reaction temperature more closely matching body temperature (about 37° C.) at which antibodies are designed to react. While such convection or radiant heating systems have been generally suitable for IHC, which is antibody-based, they are less suitable for ISH, which is nucleic acid-based and requires higher and more precise temperature control in order to denature DNA. In order to denature the DNA double helix of both the target sample and the probe so as to render them single stranded, the temperature must be raised above the melting point of the duplex, usually about 94° C. Precise temperature control is also required in ISH to effect probe hybridization at the desired stringency. The selected temperature must be low enough to enable hybridization between probe and target, but high enough to prevent mismatched hybrids from forming.

[0013] Hot air convection, conduction or radiant heat heating units typically employed with prior art automated tissue stainers do not permit the temperature of individual slides to be separately controlled. With prior art systems all of the slides are heated to the same temperature at any given time during the process. For example, U.S. Pat. Nos. 5,645, 114 and 6,180,061 to Bogen et al. disclose a dispensing assembly adapted to carry a plurality of microscope slides. Individual slide holders containing resistive heating units are provided. However, with the assembly taught by Bogen et al., all of the slides would be heated to a common temperature because no means are disclosed for separate heating controls or for shielding slides from heat generated by adjacent slides.

[0014] Other difficulties frequently encountered in both IHC and ISH testing results from the manner in which the tissues are typically preserved. The mainstay of the diagnostic pathology laboratory has been for many decades the formalin-fixed, paraffin-embedded block of tissue, sectioned

and mounted upon glass slides. Fixation in such a preservative causes cross-linking of macromolecules, both amino acids and nucleic acids. These cross-linked components must be removed in the case of ISH, to allow access of the probe to the target nucleic acid, and, in the case of IHC, to allow the antibody to recognize the corresponding antigen. "Unmasking" the antigen and/or nucleic acid is typically accomplished manually with multiple pretreatment, proteolytic digestion, and wash steps.

[0015] Prior to staining, complete removal of the paraffin is also required so that it does not interfere with antibody or probe binding. Manual deparaffinization normally is achieved by the use of two or three successive clearing reagents that are paraffin solvents such as xylene, xylene substitutes or toluene. However, new automated methods that are largely based on physical separation mechanisms are revealed in U.S. Pat. No. 6,544,798 B1 to Christensen et al., which do not require toxic solvents and are aqueous-based.

[0016] The foregoing discussion of the prior art largely derives from Richards et al. U.S. Pat. No. 6,296,809, assigned to Ventana Medical Systems, in which there is described apparatus and methods for automatically staining or treating multiple tissue samples mounted on microscope slides so that each sample can receive an individualized staining or treatment protocol even when such protocols require different temperature parameters. More specifically, there is described in the '809 patent apparatus comprising a computer controlled, bar code driven, staining instrument that automatically applies chemical and biological reagents to tissue or cells mounted or affixed to standard glass microscope slides. According to the '809 patent, a plurality of slides are mounted in a circular array on a carousel which rotates, as directed by the computer, to a dispensing location placing each slide under one of a series of reagent dispensers on a second rotating carousel positioned above the slides. Each slide receives the selected reagents (e.g. DNA probe) and is washed, mixed and/or heated in an optimum sequence and for the required period of time.

[0017] According to the '809 patent, individual slides are carried on thermal platforms radially mounted to the carousel. Temperature sensors are also mounted to the slide carousel, individually monitoring and controlling each thermal platform separately. Apparatus made in accordance with the '809 patent is available commercially from Ventana Medical Systems, of Tucson, Ariz. as the DISCOVERY® or BENCHMARK® systems.

[0018] The present invention is a modification and improvement over the prior art including the apparatus and methods described in the '809 patent. More particularly, the present invention rather than bringing the slides to the reagent, stain, and wash stations, brings the reagent, stain and wash stations to fixedly positioned slides. That is to say, in the present invention the slides are fixedly positioned in the apparatus, and the various washing, staining and reagent fluids are selectively delivered to the slides. Fixing the slides in position in the apparatus simplifies wiring to the heaters, and also eliminates the potential that a slide may be dislocated by rapid start and stop movement of the slide carousel, which, in a worst case scenario could result in a domino or train-wreck effect where one dislocated slide hits the neighboring slide causing that slide to dislocate, and so forth.

US 2003/0203493 A1

Oct. 30, 2003

3

BRIEF DESCRIPTION OF THE DRAWINGS

[0019] Further features and advantages of the present invention will be seen from the following detailed description, taken in conjunction with the accompanying drawings, wherein like numerals depict like parts, and wherein:

[0020] **FIG. 1** is a perspective view of a first embodiment of an apparatus of the present invention shown with the slide cabinet shell removed, and **FIG. 1A** is an enlarged view showing details of portions of the reagent transfer probes;

[0021] **FIG. 2** is a perspective view of the apparatus of **FIG. 1**, first embodiment shown in conjunction with a computer and other instruments with which it operates;

[0022] **FIG. 3** is a perspective view and **FIG. 3A** is a partially exploded view of details of the nozzle support portion of **FIG. 1**, first embodiment;

[0023] **FIG. 4** is an exploded view of details of the slide plate portion of **FIG. 1**, first embodiment;

[0024] **FIGS. 5 and 6** are perspective views, from the top and the bottom, respectively, of portions of the slide plate portion of **FIG. 1**, first embodiment;

[0025] **FIG. 7** is a perspective view of the reagent support portion of **FIG. 1**, first embodiment;

[0026] **FIG. 8** is a partially exploded perspective view showing two reagent bottles of **FIG. 1**, first embodiment;

[0027] **FIG. 8A** is a cross-sectional view of a reagent bottle, cap and insert, first embodiment;

[0028] **FIG. 9** is a top plan view of two reagent bottles of **FIG. 1**, first embodiment;

[0029] **FIGS. 10A-10B** are flow charts of the operation and control of **FIG. 1**, first embodiment;

[0030] **FIG. 11** is a perspective view of an alternative embodiment and apparatus of the present invention shown with the slide cabinet shell removed;

[0031] **FIG. 12** is a perspective view of the **FIG. 11** alternative embodiment shown in conjunction with a computer and other instruments with which it operates;

[0032] **FIG. 13** is a perspective view showing details of the nozzle support portion of the **FIG. 11** alternative embodiment;

[0033] **FIG. 14** is an exploded view of details of the **FIG. 11** alternative embodiment;

[0034] **FIGS. 15 and 16** are perspective views, from the top and the bottom, respectively, of portions of the slide plate portion of the **FIG. 11** alternative embodiment;

[0035] **FIGS. 17A and 17B** are front and rear perspective views of the reagent dispenser and dispenser carrier portion of the **FIG. 11** alternative embodiment;

[0036] **FIG. 18** is a perspective view showing details of the reagent dispenser activator portion of the **FIG. 11** alternative embodiment; and

[0037] **FIGS. 19A and 19B** are flow charts of the operation and control of the **FIG. 11** alternative embodiment.

DETAILED DESCRIPTION OF THE INVENTION

[0038] Referring now in detail to the drawings wherein like parts are designated by like reference numerals throughout, there is illustrated in **FIG. 1** a perspective view of the molecular pathology apparatus according to a first embodiment of the present invention which is designated generally by reference numeral **10**. For the purposes of clarity, several of the reagent bottles, as well as the cabinet shell, and liquid and air supply tubing and electrical wiring are omitted from the drawings. Apparatus **10** is designed to automatically stain or otherwise treat tissue mounted on microscope slides with nucleic acid probes, antibodies, and/or other reagents in a desired sequence, time and temperature. Tissue sections so stained or treated are then to be viewed under a microscope by a medical practitioner who reads the slide for purposes of patient diagnosis, prognosis, or treatment selection.

[0039] In the first embodiment, apparatus **10** functions as one component or module of a system **12** (**FIG. 2**) which also comprises a host computer **14** preferably a personal computer, monitor **16**, keyboard **18**, mouse **20**, bulk fluid containers **22**, waste container **23** and related equipment. Additional staining modules or other instruments may be added to system **12** to form a network with computer **14** functioning as a server. Alternatively, some or all of these separate components could be incorporated into apparatus **10** making it a stand-alone instrument.

[0040] Referring also to **FIGS. 3, 3A** and **4-7**, as set forth in greater detail below, a plurality of slide platforms **50** (**FIGS. 4, 5**) are mounted radially about a center point **32** of drawer **34** (**FIG. 1**) upon which standard glass slides **60** with tissue samples may be placed. Drawer **34** is slidably mounted in housing **30** on rails **40** or the like. The temperature of each slide may be individually controlled by means of sensors and a microprocessor, i.e. as taught in the above-mentioned '809 patent.

[0041] Each of the slide platforms **50** is connected through individual wires to a multiplexer (not shown) which is then in turn connected to a microprocessor (not shown). A feature and advantage of the present invention which results from fixedly mounting the slide platforms in drawer **34** is that each of the heaters and thermal sensors may be hardwired thereby eliminating the need for a slip ring assembly or rotor couplings, as well as complex stepping motors, etc. for locating and positioning a rotating slide carousel as required in prior art devices. Also, the possibility that a slide or slides may be shifted or dislocated during rapid start and stop rotation of the slide carousel is eliminated.

[0042] In one embodiment, a plurality of slots or channels are formed on the top surface of each of the slide heaters, i.e. the interface surface between the slide heater and the slide, for gathering and venting gas bubbles as may form during heating, i.e. in accordance with co-pending U.S. application Ser. No. 09/953,417, filed Sep. 11, 2001, and assigned to the common assignee, which disclosure is incorporated herein by reference.

[0043] Referring also to **FIGS. 1, 2, 5** and **6**, drawer **34** supports a slide support tray **33** which in turn supports a circular pan **35** having a peripheral wall **36** serving as a splash guard, a peripheral trough **37** and a central drain **38**, i.e. at center point **32**, both connected to drain lines **39** which

US 2003/0203493 A1

Oct. 30, 2003

4

in turn are connected to waste container **23**. Drawer **34** is slidably mounted in housing **30** on rails **40**. Rails **40**, in a preferred embodiment, comprise three piece telescoping rails so that the drawer **34** may be slid clear of housing **30** to permit access to all of the slide platforms **50** for slide loading and removal. A damping means such as a pneumatic means, electromotive means, mechanical spring damper or the like preferably is provided to smooth movement of the drawer whereby to avoid possible dislodging of slides, particularly when the drawer is closed. Slide support tray **33** is supported on a lift mechanism such as pneumatic cylinders **52** (see FIG. 1), which automatically index to permit the slide support tray **33** to move up and down so that the slide support tray **33** and circular pan **35** may be dropped to permit wall **36** to clear the nozzle support **100** when the drawer is slid in and out of the apparatus.

[0044] Slide drawer **34** is divided into thirty-five equal pie-shaped sections **70**. Thirty of the pie-shaped sections **70** are occupied by slide platforms **50** while the five remaining pie-shaped sections **70A** (FIG. 4) at the rear of the drawer are devoid of slide platforms **50**. In other words, a row of thirty slide platforms **50** are radially mounted on drawer **34** and evenly spaced from one another, except at the ends of the row.

[0045] However, the invention is not limited to thirty active slide locations, and more or fewer slide locations may be employed. An alternative embodiment may be implemented by aligning the platforms **50** linearly, which results in potentially limitless number of platforms.

[0046] Referring to FIGS. 1 and 3, a nozzle support **100** is concentrically and rotatably mounted above slide drawer **34**. Nozzle support **100** is mounted on a shaft (not shown) supported by a bridge **110**, and driven by a computer controlled stepping motor and drive belt (not shown), and rotates plus or minus approximately 180° from a home position **104** at the rear of the drawer. The computer controlled stepper motor and drive belt are conventional in this art. Accordingly, details are omitted for the sake of clarity.

[0047] Nozzle support **100** carries the various slide treatment stations, other than the reagent dispensing location. Thus, nozzle support **100** carries dual rinse nozzle block **102**, volume adjust/stringency block **103**, Liquid Coverslip™ evaporation inhibitor liquid application block **105**, vortex mixer air jet block **106**, jet drain **108**, and the like, all for preparing a slide for staining, stain removal, and the like, and to clear bar codes (not shown) carried on the slides, and a bar code reader **109**, all as described in detail in U.S. Pat. Nos. 5,595,707; 5,650,327; 5,654,199; or 5,654,200 to Copeland et al, which disclosures are incorporated herein by reference. In other words, nozzle support **100** carries all of the functions for slide preparation, cleaning, reagent mixing, Liquid Coverslip™ application, etc. other than reagent application, as described, e.g. in the '707 patent to Copeland et al., plus wash stations **121**, **122** for the reagent application probes as will be described in detail below.

[0048] Preferably, but not necessarily, the various rinse nozzle blocks, vortex mixer air jet blocks, jet drain, etc. are arranged adjacent to one another so that the nozzle support **100** may be indexed and advanced in a "lock-step" manner to sequentially treat a slide according to an accepted protocol. For example, jet drain **108** may be arranged immediately adjacent rinse nozzle blocks **102** so that nozzle support

100 may be advanced in "lock step" manner past a selected slide, and the slide rinsed and fluid stripped, etc. Also, if desired, vortex mixer air jet blocks **106** may be oriented to impinge simultaneously on two adjacent slides.

[0049] For the sake of clarity, fluid and air supply tubing for the several slide treatment stations have been omitted from the drawings. It will be understood, however, that the fluid and air supply tubing are made long enough to permit the valve plate to rotate plus or minus approximately 190° from a home position at the rear of the apparatus so that each slide treatment station can reach each slide **60**. A pair of wash stations **121**, **122** spaced two thirty-fifths of a revolution (approximately 20°) apart as will be described in detail hereinafter, are also attached to and radially extend beyond the periphery of the nozzle support **100**, and rotate with the nozzle support **100**.

[0050] Reagent support **300** is fixedly mounted to bridge **110** vertically above nozzle support **100**, which arch in turn is fixedly mounted within housing **30**. A plurality of reagent bottles **302** are removably mounted within recesses **304** formed equally spaced adjacent the periphery of reagent support **300**. In the illustrated embodiment, a total of thirty-five reagent bottles are mounted on the reagent support **300**, spaced approximately one thirty-fifth (approximately 10°) apart.

[0051] The reagents may include any chemical or biological material conventionally applied to slides including nucleic acid probes or primers, polymerase, primary and secondary antibodies, digestion enzymes, pre-fixatives, post-fixatives, readout chemistry, counterstains, and the like.

[0052] Referring also to FIG. 8, the reagent bottles **302** each comprise a cylindrical hollow body **305** closed at the bottom end by an integrally formed bottom wall. Preferably, the inside bottom wall of each bottle is cone shaped, i.e. as shown in phantom at **303** to facilitate reagent pick-up by reagent transfer probes as will be described in detail below. Each bottle **302** includes an integrally formed bracket **306** which serves to maintain the bottles **304** at a desired height in reagent support **300**, and which may serve also to permit the stringing together of a plurality of like bottles **302**. Accordingly, each bracket **306** includes a hinge element **308** for cooperating with a hinge element **310** of an adjacent bottle **302**. In the illustrated embodiment, hinge elements **308** and **310** are shown as conventional pin-hinges in which the upper hinge **310** includes a pin **312** which fits into the lower hinge **308**, i.e. similar to a conventional door hinge. However, bottles **302** may be hinged together in a variety of ways.

[0053] Bracket **306** preferably includes a flat surface **314** upon which is carried a bar code **316** for identifying the contents of the bottle **302**. Bottles **302** also include an insert **318** having a tapered top surface **320** and inlet **319** fitted in the top end of the bottles for locating a reagent transfer probe **328** as will be described in detail hereinafter, and a cap **322** which may be either twist or snap-fitted to the bottle **302** for sealing the bottle **302**.

[0054] Probe **328** is tapered at a lower end to fit closely in tapered conical bottom **303** of bottle **302**. A vent **321** is formed in insert **318** for equalizing air pressure as reagent is removed. Cap **322** includes a tapered inner surface and plug **323** for sealing inlet **319**.

US 2003/0203493 A1

Oct. 30, 2003

5

[0055] Making brackets 306 attachable to one another permits one to assemble a chain of reagents for use, and also to remove the chain of reagents so that the reagents may be refrigerated, for example, overnight when not in use.

[0056] Referring next to FIGS. 7, 8 and 9, the side walls 324 of brackets 306 are tapered so that a pie-shaped space 326 is formed between two bottles when two bottles are fastened together in a string, and mounted in recesses 304 in the reagent support 300, thereby exposing holes 328 formed through reagent support 300. Holes 328 are formed in the same concentric circle as recesses 304, and are spaced equidistant between adjacent recesses 304. The purpose of pie-shaped spaces 326 and holes 328 is to provide clearance for reagent transfer probes 402, 404 as will be described in detail below.

[0057] Referring again to FIG. 1, an arm 400 is rotatably mounted on arch 405 concentrically above reagent support 300, and carries a pair of reagent transfer probes 402, 404 located at the distal end of arm 400 and spaced approximately 10° apart. Arm 400 also carries a bar code reader 406 for reading bar codes 316 on the reagent bottles. Arm 400 is rotatably driven by a computer driven stepping motor (not shown), and rotates plus or minus approximately 185° in either direction from a home position 410.

[0058] Reagent transfer probes 402 and 404, which are identical to one another, preferably comprise automatic pipette metering/dispensing pick-up devices designed to aspirate or "sip" reagent from a reagent bottle, move to a slide, and then "spit" or deposit the reagent onto the slide. "Sip" and "spit" automatic pipette/metering dispensing pick-up devices are described in published PCT Application No. PCT/US99/04379, which disclosure is incorporated herein by reference. Reagent transfer probes 402 and 404 are carried on the distal end of arm 400 and are spaced from one another so that when one of the probes, e.g. probe 402 is located centrally over a slide 60, the other reagent transfer probe 404 may be centrally positioned over one of the two probe wash stations 121 or 122. Pneumatic cylinders 403a, 403b selectively raise and lower probes 402 and 404 into one of the following positions: a raised transport position above the tops of the bottles 302 where the arm 400 is free to rotate; a reagent drawing position wherein one of the probes is inserted into a selected reagent bottle 302 wherein a measured amount of reagent may be drawn into the probe; a reagent dispensing position wherein a reagent transfer probe containing reagent is disposed in the pie-shaped space 326 between two reagent bottles, above a selected slide to dispense reagent thereon; and a cleaning position wherein the other probe, i.e. the probe not being used to dispense reagent, is operatively disposed in one of probe washing stations 121 or 122 which straddle the slide being dispensed upon. While the apparatus of the present invention could be made with only a single reagent transfer probe, providing two spaced reagent transfer probes improves cycle speed since reagent metering may be accomplished using one of the two reagent transfer probes while the other of the two reagent transfer probes is going through the wash cycle as will be described below. That is to say, while one of the reagent transfer probes, e.g. reagent transfer probe 402 is dispensing reagent onto a slide, the other reagent transfer probe, i.e. idle reagent transfer probe 404 may be lowered to a probe wash station 121 where the idle reagent transfer probe may be rinsed inside and out at the same time.

[0059] Referring to FIGS. 10A and 10B, the overall process is as follows:

[0060] A plurality of specimen-bearing slides 60 are mounted on the slide platforms 50, selected reagent bottles 302 mounted in the reagent support 300, the slide drawer is closed and the slide and reagent bar codes are read. The computer calculates the master protocol and then downloads the run steps for the entire run, the nozzle support 100 is indexed to the first slide, and the slide is washed and prepared for staining or other treatment in accordance with the pre-programmed run steps by advancing the nozzle support 100 in "lock-step" manner. In the meanwhile, probe arm 400 is rotated to the appropriate reagent bottle 302, one of the two reagent transfer probes 402 or 404 is indexed over the selected reagent bottle, and the probe lowered to aspirate a measured amount of the desired reagent. The reagent-containing transfer probe is then raised, and the arm 400 moved to the selected slide where the loaded reagent transfer probe is lowered to just over the slide, and the reagent dispensed on the slide. In the meanwhile, the idle reagent transfer probe is lowered into one of the washing stations 121 or 122, wherein the reagent transfer probe is washed inside and out. Both reagent transfer probes 402 and 404 are then raised, and the process repeated, but using the reagent transfer probe just cleaned in the previous step to aspirate and dispense reagent onto the next slide. As before, simultaneously with dispensing the reagent onto the slide as in the previous case, the idle reagent transfer probe is washed while the active reagent transfer probe is dispensing reagent onto the new slide.

[0061] The foregoing steps are repeated until all of the slides are processed. For convenience, in the illustrated embodiment, the dwell time at each slide station is six and two-thirds seconds. This comes from dividing a four minute cycle time into thirty-six time spaces, one time space for each of the thirty slide positions plus five blank slide positions for overtravel of the slide support, plus one "virtual" slide position for returning the nozzle support 100 from the last slide position to the first slide position. The virtual slide position allows the nozzle support 100 to return to the other end of its travel range in an uninterrupted fashion.

[0062] The staining algorithm used on the aforesaid Ventana systems avoids scheduling problems associated with random access methods by using a "lock step" method. The lock step algorithm requires that the nozzle support 100 which holds the processing functions be rotated one slide position index every "n" seconds, termed the slide index time. The slide index time is preferably as short as possible but long enough that the function that requires the longest time can be completed within the index time. In the embodiments of the inventions herein, "n" is six and two-thirds seconds. Index times are usually on the order of several seconds. The time for one complete rotation of the nozzle support 100, termed the fundamental incubation period, will then be "n" times the number of slide positions, including blank and virtual slide positions. (For example, if the slide index time is six seconds and there are twenty slide positions, the incubation time period will be 120 seconds or two minutes.)

US 2003/0203493 A1

Oct. 30, 2003

6

[0063] Throughout the entire run the nozzle support **100** is indexed one slide position every "n" seconds. After the index, the system checks the schedule to see if any of the slides at each of the processing stations require the function of that station. For example, if the slide at the washing station is scheduled for washing, that slide is washed. Similarly if the slide at the reagent application station is scheduled for the application of a new reagent, then the new reagent is applied.

[0064] The above-described invention has several advantages over the prior art. For one, making the slide plate fixed in position eliminates the possibility of a slide being dislocated (and the sample dislodged) during the rapid start-stop rotational movement of a conventional rotating slide carousel. Also, employing two transfer syringes insures better cleaning of transfer syringes without increasing cycle time.

[0065] Also, since none of the moving elements, i.e. nozzle support **100** and probe support arm **400** need travel more than approximately 190° in either direction, all electrical connections, and air and fluid connections can be achieved without the need for slip ring or rotary connections, since the hoses and wires are quite capable of taking twistings of 190° plus.

[0066] The instrumentation described herein may or may not have the ability to continuously rotate the nozzle support. The nozzle support **100** may need to return to a starting position before rotation has exceeded 360 degrees. This may also be required when the slides are rotated on a carousel and the processing functions are fixed above the slides. Similarly, other non-rotating designs are possible such as linear or two dimensional configurations. In these cases there will be a requirement to move the slides or processing functions back to the original starting position during the staining run. In most cases it is likely that the time required to do this will exceed the index time which violates the fundamental requirement of the lock step algorithm. The lock step algorithm can still be utilized through the concept of the "virtual slide" previously mentioned. The virtual slide is added to the total number of actual slide positions so that the index time period assigned to the virtual slide may be used to move the slides or processing stations back to the starting position. Thus accurate and predictable incubation times are maintained.

[0067] While one embodiment of the invention has been described, the invention is susceptible to modification. For example, instead of using one or a pair of transfer syringes on an overhead arm, the reagent carousel could carry a plurality of micro-delivery reagent fluid dispensers such as described in U.S. Pat. Nos. 6,045,759; 6,416,713; or 6,192,945. Moreover, while the use of individually heated thermal platforms is preferred, the slides may be heated using conventional heating techniques.

[0068] Referring to FIGS. 11-19, there is illustrated a second embodiment of the present invention. FIG. 11 is a perspective view of a molecular pathology apparatus according to the second embodiment which is designated generally by reference numeral **1000**. For the purposes of clarity, all but one of the reagent dispensers and dispenser carriers, as well as the cabinet shell, and liquid and air supply tubing and electrical wiring are omitted from the drawings. Apparatus **1000** is designed to automatically stain or otherwise treat tissue mounted on microscope slides with nucleic acid

probes, antibodies, and/or other reagents in a desired sequence, time and temperature. Tissue sections so stained or treated are then to be viewed under a microscope by a medical practitioner who reads the slide for purposes of patient diagnosis, prognosis, or treatment selection.

[0069] In one embodiment, apparatus **1000** (FIG. 12) functions as one component or module of a system which also comprises a host computer **1014** preferably a personal computer, bulk fluid containers **1022**, waste container (not shown) and related equipment. Additional staining modules or other instruments may be added to the system to form a network with computer **1014** functioning as a server. Alternatively, some or all of these separate components could be incorporated into apparatus **1000** making it a stand-alone instrument.

[0070] Referring also to FIGS. 14, 15 and 18, as set forth in greater detail below, a plurality of slide platforms **1050** are mounted radially about a center point **1032** of slide support assembly **1099** upon which standard microscope glass slides **1060** with tissue samples may be placed. Drawer **1034** is slidably mounted in housing **1030** on rails **1040** or the like. The temperature of each slide may be individually controlled by means of temperature sensors and a micro-processor, i.e. as taught in the above-mentioned '809 patent.

[0071] As in the case of the first embodiment, each of the slide platforms **1050** is connected through individual wires to a multiplexer (not shown) which is then in turn connected to a microprocessor (not shown). Also, as in the case of the first embodiment, a plurality of slots or channels are formed on the top surface of each of the slide heaters, i.e. the interface surface between the slide heater and the slide, for gathering and venting gas bubbles as may form during heating, i.e. in accordance with co-pending U.S. application Ser. No. 09/953,417, filed Sep. 11, 2001, and assigned to the common assignee, which disclosure is incorporated herein by reference.

[0072] Referring to FIGS. 14-16, drawer **1034** supports a slide support assembly **1099** which is comprised of a slide support **1033** which in turn supports a circular pan **1035** having a peripheral wall **1036** serving as a splash guard, a peripheral trough **1037** and a central drain **1038**, i.e. at center point **1032**, both connected to drain lines **1039** which in turn are connected to waste container **1023**. Drawer **1034** is slidably mounted in housing **1030** on rails **1040**. Rails **1040**, in a preferred embodiment, comprise three-piece telescoping rails so that the drawer **1034** may be slid clear of housing **1030** to permit access to all of the slide platforms **1050** for slide loading and removal. A damping means such as a pneumatic means, electromotive means, mechanical spring damper or the like (not shown) preferably is provided to smooth movement of the drawer whereby to avoid possible dislodging of slides, particularly when the drawer is closed. Slide support assembly **1099** is supported on a lift mechanism such as pneumatic cylinders **1052** (see FIG. 11), which automatically index to permit the slide support assembly **1099** to move up and down so that the slide support plate **1033** and circular pan **1035** may be dropped to permit wall **1036** to clear the nozzle support **1100** when the drawer is slid in and out of the apparatus.

[0073] Slide support assembly **1099** is allocated into thirty-five equal pie-shaped sections **1070**. Thirty of the pie-shaped sections **1070** are occupied by slide platforms

US 2003/0203493 A1

Oct. 30, 2003

7

1050 while the five remaining pie-shaped sections **1070A** (**FIG. 15**) at the rear of the drawer are devoid of slide platforms **1050**. In other words, a row of thirty slide platforms **1050** are radially mounted within slide support assembly **1099** and evenly spaced from one another, except at the ends of the row.

[0074] However, the invention is not limited to thirty active slide locations, and more or fewer slide locations may be employed. An alternative embodiment may be implemented by aligning the platforms **1050** linearly, which results in potentially limitless number of platforms.

[0075] Referring to **FIGS. 11, 14** and **18**, a nozzle support **1100** is concentrically and rotatably mounted above slide support assembly **1099**. Nozzle support **1100** is mounted on a shaft **1113** which in turn is rotatably mounted on a bridge **1112**, and driven by a computer controlled stepping motor and drive belt (not shown), and rotates plus or minus approximately 190° from a home position at the rear of the drawer. The computer controlled stepper motor and drive belt are conventional in this art. Accordingly, details are omitted for the sake of clarity.

[0076] With respect to **FIG. 13**, nozzle support **1100** carries the various slide treatment stations, other than the reagent dispensing station. Thus, nozzle support **1100** carries dual rinse nozzle block **1102**, volume adjust/stringency block **1103**, Liquid Coverslip™ evaporation inhibitor liquid application block **1105**, vortex mixer air jet block **1106**, jet drain **1108**, and the like, all for preparing a slide for staining, stain reagent removal, and the like, and to clear the bar codes (not shown) carried on the slides, and a bar code reader **1109**, all as described in detail in U.S. Pat. No. 5,595,707 to Copeland et al, which disclosure is incorporated herein by reference. In other words, nozzle support **1100** carries all of the functions for slide preparation, cleaning, reagent mixing, Liquid Coverslip™ application, etc. other than reagent application, as described in the '707 patent to Copeland et al.

[0077] Preferably, but not necessarily, the various rinse nozzle blocks, vortex mixer air jet blocks, jet drain, etc. are arranged adjacent to one another so that the nozzle support **1100** may be indexed and advanced in a "lock-step" manner to sequentially treat a selected slide according to an accepted protocol. For example, jet drain **1108** may be arranged immediately adjacent rinse nozzle blocks **1106** so that nozzle support **1100** may be advanced in "lock step" manner past a selected slide, and the slide rinsed and fluid stripped, etc. Also, if desired, vortex mixer air jet blocks **1106** may be oriented to impinge simultaneously on two adjacent slides.

[0078] For the sake of clarity, fluid and air supply tubing for the several slide treatment stations have been omitted from the drawings. It will be understood, however, that the fluid and air supply tubing are made long enough to permit the valve plate to rotate plus or minus approximately 190° from a home position at the rear of the apparatus so that each slide treatment station can reach each slide **1060**.

[0079] With respect to **FIGS. 11** and **14**, reagent support **1300** is fixedly mounted to a cage **1110** vertically above nozzle support **1100**, which cage in turn is rotatably mounted for rotation on a shaft **1113**, which in turn is driven by a stepper motor and belt (not shown). A plurality of reagent dispensers **1302** are removably mounted equally spaced adjacent the periphery of reagent support **1300**. In the

illustrated embodiment, a total of thirty-five reagent dispensers are carried by the reagent support **1300**, spaced approximately one thirty-fifth (approximately 10°) apart. Preferably, the reagent dispensers are mounted on curved dispenser carriers **1303**, which in turn are mounted on reagent support **1300** (see **FIG. 17A**).

[0080] Curved dispenser carrier **1303** permits a lab worker to assemble a kit of reagent dispensers for use, and also to remove the kit of reagent dispensers so that the reagents may be refrigerated, for example, overnight when not in use.

[0081] The reagents may include any chemical or biological material conventionally applied to slides including nucleic acid probes or primers, polymerase, primary and secondary antibodies, digestion enzymes, pre-fixatives, post-fixatives, readout chemistry, counterstains, and the like.

[0082] Referring in particular to **FIGS. 17A** and **17B**, the reagent dispensers **1302**, are shown mounted on dispenser carrier **1303**.

[0083] Referring to both **FIGS. 17A** and **17B**, each of the dispensers **1302** carries a plate **1307** upon which may be mounted a bar code which may be read by a bar code reader (not shown).

[0084] Referring also to **FIG. 18**, a hammer or piston **1400** is carried by an arm **1402** which is mounted on shaft **1113** for rotation with the shaft. Hammer **1400** is keyed to move with the nozzle support **1100**, and is vertically and concentrically operatively aligned over the reagent dispensers **1302**. Hammer or piston **1400** comprises a servo or piston **1404** for moving vertically into engagement with the top of a selected reagent dispenser, and force a metered quantity of reagent from the dispenser i.e. as explained in detail in U.S. Pat. No. 6,192,945. Thus, in order to dispense a selected reagent on a selected slide, the nozzle support **1100** is rotatably moved to a dispense position vertically over the selected slide which had been previously prepared, e.g. washed, etc., by the treatment stations carried on the nozzle support **1100**. Since the hammer is keyed to move with the nozzle support **100**, there is no time wasted in moving the hammer or piston, and the hammer or piston is vertically aligned. A particular feature and advantage of the present invention is that the reagent support **1300** requires neither electrical nor plumbing connections. Thus, the reagent support **1300** is free to rotate in any direction, without limitation.

[0085] Referring to **FIGS. 19A** and **19B**, the overall process is as follows:

[0086] A plurality of specimen-bearing slides **1060** are mounted on the slide platforms **1050**, and selected reagent dispensers **1302** are mounted on the reagent support **1300**. The slide drawer is closed and the slide and reagent bar codes are read. The computer calculates the master protocol and then downloads the run steps for the entire run, the nozzle support **1100** and hammer or piston **1400** are indexed to the first slide, and the slide is washed and prepared for staining or other treatment in accordance with the pre-programmed run steps by advancing the nozzle support **1100** in "lock-step" manner. In the meanwhile, reagent support **1300** is rotated to locate a selected reagent dispenser **1302** over the selected slide **1060**, and the hammer or piston **1400** activated

US 2003/0203493 A1

Oct. 30, 2003

8

to dispense a measured amount of the desired reagent. The process is repeated for a second selected slide, and so forth.

[0087] Still other changes may be made without departing from the spirit and scope of the invention.

What is claimed is:

1. An automatic slide processing apparatus comprising:

- (a) a slide support;
- (b) a reagent support;
- (c) a nozzle support; and
- (d) a reagent dispenser,

wherein the slide support and the reagent support are operatively fixedly positioned, and the nozzle support is selectively rotatably movable relative to the slide support and the reagent support.

2. An apparatus as claimed in claim 1, wherein the slide support carries a plurality of spaced slide support platforms.

3. An apparatus according to claim 2, wherein said slide support platforms include heaters and/or temperature sensors.

4. An apparatus as claimed in claim 1, wherein said slide support includes at least one liquid drain.

5. An apparatus according to claim 1, wherein said slide support is slidably mounted in the apparatus to permit loading and unloading of slides in the slide support.

6. An apparatus according to claim 5, wherein said slide support is slidably mounted on rails.

7. An apparatus according to claim 6, and further including a damper for damping smoothing movement of the rails.

8. An apparatus according to claim 1, wherein said slide support is vertically adjustably supported on a lift mechanism.

9. An apparatus according to claim 1, wherein said reagent dispenser is selectively moveable relative to the reagent support.

10. An apparatus according to claim 9, wherein said reagent dispenser comprises robotic dispensing pipettes.

11. An apparatus according to claim 10, wherein said robotic dispensing pipettes are vertically moveable between an operating position and a transport position.

12. An apparatus according to claim 9, wherein said reagent dispenser comprises two spaced robotic dispensing pipettes.

13. An apparatus according to claim 1, wherein the nozzle support carries at least one vortex air jet or jet drain.

14. An apparatus according to claim 1, wherein the nozzle support carries at least one applicator for applying a cover fluid to the slide.

15. An apparatus according to claim 1, wherein the nozzle support is rotatably moveable plus or minus approximately 180° from a home position.

16. An apparatus according to claim 9, wherein said reagent dispenser is rotatably moveable plus or minus approximately 185° from a home position.

17. An apparatus according to claim 1, and further comprising a slide bar code reader carried on the nozzle support and/or carried with the reagent dispenser.

18. An apparatus according to claim 1, and further comprising a processor for controlling movement of the nozzle support, and the reagent dispenser.

19. An apparatus according to claim 1, and further comprising a dispenser wash station mounted on the nozzle support.

20. An apparatus according to claim 19, and comprising two dispenser wash stations mounted spaced from one another on the nozzle support.

21. An apparatus according to claim 1, wherein the slide supports are fixedly positioned relative to the reagent dispenser.

22. A method for processing a plurality of slides each having biological samples thereon comprising the steps of:

- (a) preparing a first slide for biological treatment with a reagent;
- (b) moving a reagent dispenser to a selected reagent container;
- (c) drawing a pre-selected volume of reagent from the reagent container into the reagent dispenser;
- (d) moving the reagent dispenser to the first slide;
- (e) dispensing said pre-selected volume of reagent from the reagent dispenser onto the first slide;
- (f) preparing a second slide for treatment with a reagent;
- (g) cleaning the reagent dispenser;
- (h) moving a reagent dispenser to a selected reagent which may be the same or different from the reagent of step (b);
- (i) drawing a pre-selected amount of reagent from the reagent container selected in step (h) into the reagent dispenser;
- (j) moving the reagent dispenser to said second slide;
- (k) dispensing said pre-selected volume of reagent selected in step (h) from the reagent dispenser onto said second slide;
- (l) cleaning the reagent dispenser; and
- (m) repeating steps (h)-(l).

23. The method of claim 22, wherein two reagent dispensers are provided, and including the step of cleaning one of the reagent dispensers while the other reagent dispenser is employed to draw and dispense reagent onto a selected slide.

24. A method according to claim 22, wherein said reagent dispenser comprises a robotic syringe, and reagent is taken up by aspiration.

25. An automatic slide processing apparatus comprising:

- (a) a slide support;
- (b) a reagent support;
- (c) a nozzle support; and
- (d) a reagent dispenser,

wherein the slide support is operatively fixedly positioned, and the nozzle support and reagent support are selectively independently movable relative to the slide support.

26. An apparatus as claimed in claim 25, wherein the slide support carries a plurality of spaced slide support platforms.

27. An apparatus according to claim 26, wherein said slide support platforms include heaters and/or temperature sensors.

28. An apparatus as claimed in claim 25, wherein said slide support includes at least one liquid drain.

29. An apparatus according to claim 25, wherein said slide support is slidably mounted in the apparatus to permit loading and unloading of slides in said slide support.

US 2003/0203493 A1

Oct. 30, 2003

9

30. An apparatus according to claim 29, wherein said slide support is slidably mounted on rails.

31. An apparatus according to claim 30, and further including a damper for damping smoothing movement of the rails.

32. An apparatus according to claim 30, wherein said slide support is vertically adaptably supported on a lift mechanism.

33. An apparatus according to claim 29, wherein a reagent dispenser activator is selectively rotatably moveable relative to the reagent support.

34. An apparatus according to claim 33, wherein said reagent dispenser activator is fixed to move in synchronization with said nozzle support.

35. An apparatus according to claim 34, wherein said reagent dispenser activator comprises a hammer or piston.

36. An apparatus according to claim 35, wherein the nozzle support carries at least one vortex air jet and/or jet drain.

37. An apparatus according to claim 25, wherein the nozzle support carries at least one applicator for applying a cover fluid to the slide.

38. An apparatus according to claim 25, wherein the nozzle support is rotatably moveable plus or minus approximately 180° from a home position.

39. An apparatus according to claim 25, wherein said reagent support is rotatably moveable in either direction from a home position.

40. An apparatus according to claim 25, and further comprising a slide bar code reader carried on the nozzle support.

41. An apparatus according to claim 25, and further comprising a reagent bar code reader operatively positioned relative to said reagent support.

42. An apparatus according to claim 25, and further comprising a processor for controlling movement of the nozzle support and reagent dispenser.

43. A method for processing a plurality of slides each having biological samples thereon comprising the steps of:

- (a) preparing a first fixedly positioned slide for biological treatment with a reagent;
- (b) moving a selected reagent dispenser to the first slide;
- (c) dispensing a pre-selected volume of reagent from the reagent dispenser onto the first slide;
- (d) preparing a second fixedly positioned slide for treatment with a reagent;
- (e) moving a selected reagent dispenser which may be the same or different from the reagent dispenser of step (b) to the second slide;
- (f) dispensing a pre-selected volume of reagent from the reagent dispenser onto said second slide; and
- (g) repeating steps (d)-(f).

44. A method according to claim 43, wherein a reagent dispenser activator is moved independently of said reagent dispensers.

45. An automatic slide processing apparatus comprising:

- (a) a slide support;
- (b) heating elements for heating the slides;
- (c) a nozzle support having nozzles for applying liquids, said nozzle support and said slide support moving relative to one another such that the nozzles may apply liquids to the slides;

(d) a reagent support; and

(e) a reagent dispenser wherein said reagent dispenser is operative to directly access the slide support.

46. An apparatus as claimed in claim 45, wherein the slide support carries a plurality of spaced slide support platforms.

47. An apparatus as claimed in claim 45, wherein said slide support includes at least one liquid drain.

48. An apparatus according to claim 45, wherein said slide support is slidably mounted in the apparatus to permit loading and unloading of slides in the slide support.

49. An apparatus according to claim 48, wherein said slide support is slidably mounted on rails.

50. An apparatus according to claim 49, and further including a damper for damping smoothing movement of the rails.

51. An apparatus according to claim 45, wherein said slide support is vertically adjustably supported on a lift mechanism.

52. The apparatus according to claim 45, wherein said reagent dispenser is selectively moveable relative to the reagent support.

53. An apparatus according to claim 52, wherein said reagent dispenser comprises at least one robotic dispensing pipette.

54. An apparatus according to claim 53, wherein said robotic dispensing pipette(s) is/are vertically moveable between an operating position and a transport position.

55. An apparatus according to claim 45, wherein said reagent dispenser comprises two spaced robotic dispensing pipettes.

56. An apparatus according to claim 45, wherein the nozzle support carries at least one vortex air jet or jet drain.

57. An apparatus according to claim 45, wherein the nozzle support carries at least one applicator for applying a cover fluid to the slide.

58. An apparatus according to claim 45 wherein the nozzle support is movable relative to the slide support.

59. An apparatus according to claim 58, wherein the nozzle support is rotatably moveable plus or minus approximately 180° from a home position.

60. An apparatus according to claim 45, wherein said reagent dispenser is rotatably moveable plus or minus approximately 185° from a home position.

61. An apparatus according to claim 45, and further comprising a slide bar code reader carried on the nozzle support and/or carried with the reagent dispenser.

62. An apparatus according to claim 45, and further comprising a microprocessor for controlling movement of the nozzle support, reagent support and the reagent dispenser.

63. An apparatus according to claim 52, and further comprising a dispenser wash station mounted on the nozzle support.

64. An apparatus according to claim 62, and comprising two dispenser wash stations mounted spaced from one another on the nozzle support.

65. An apparatus according to claim 45, wherein the slide supports are fixedly positioned relative to the reagent dispenser.

* * * * *